

FIG. 2

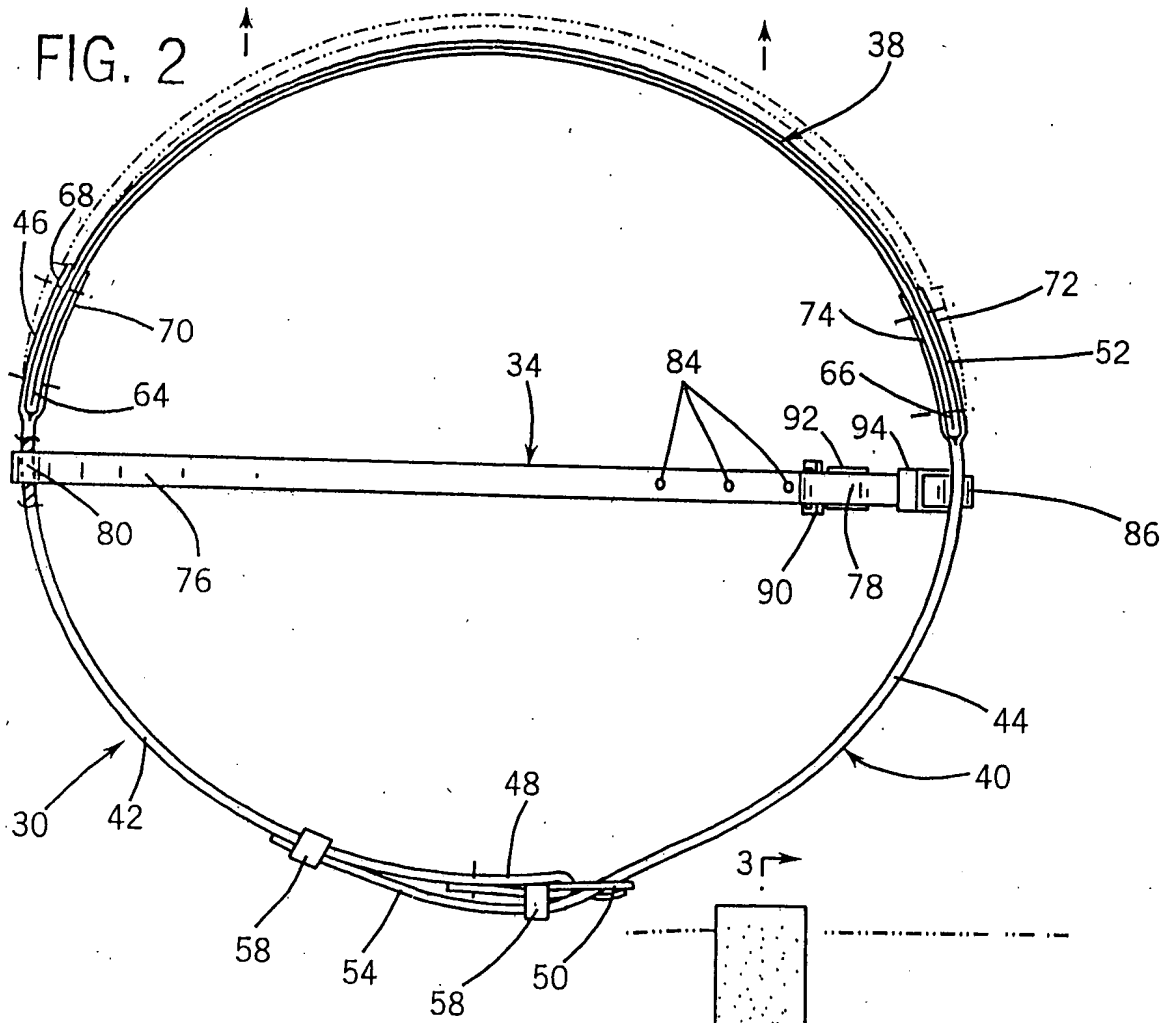


FIG. 4

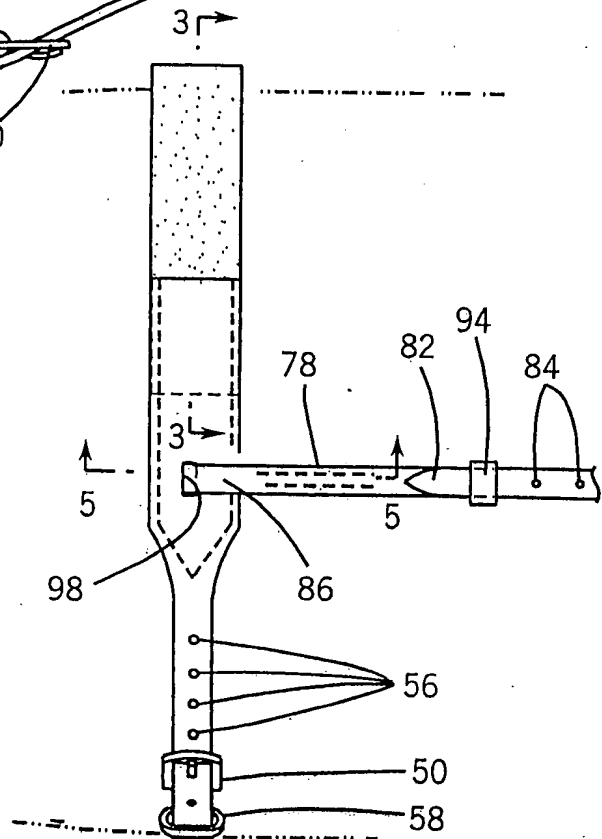
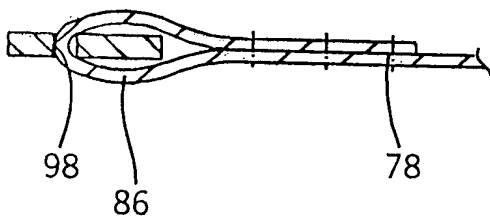


FIG. 5



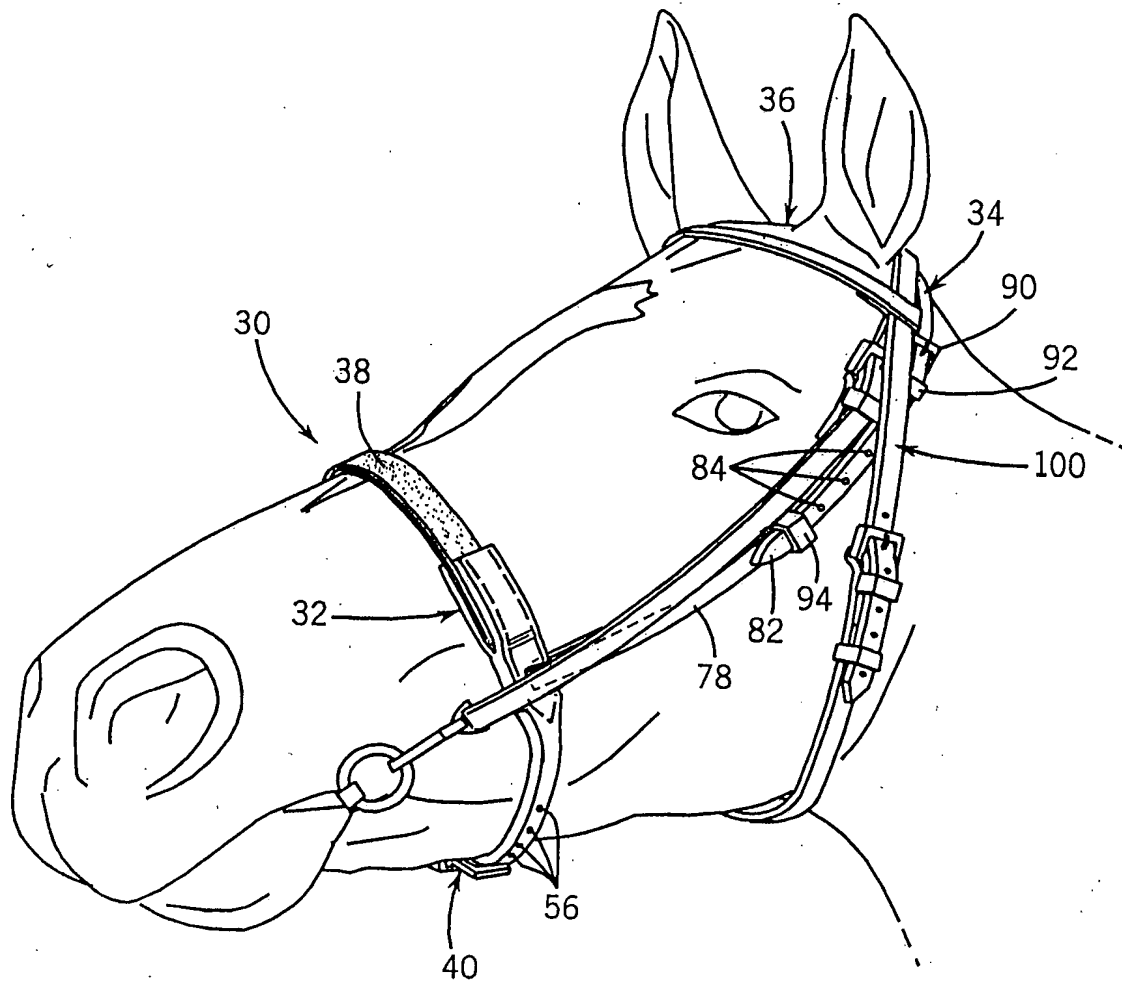


FIG. 6



FIG. 10

FIG. 10 is a side view of a medical device assembly. The assembly includes a vertical shaft (156) and a horizontal shaft (176). The vertical shaft (156) has a textured upper section and a flared lower section. The horizontal shaft (176) has a pointed tip (174) and a rectangular component (184). A circular component (164) is located at the junction of the two shafts.

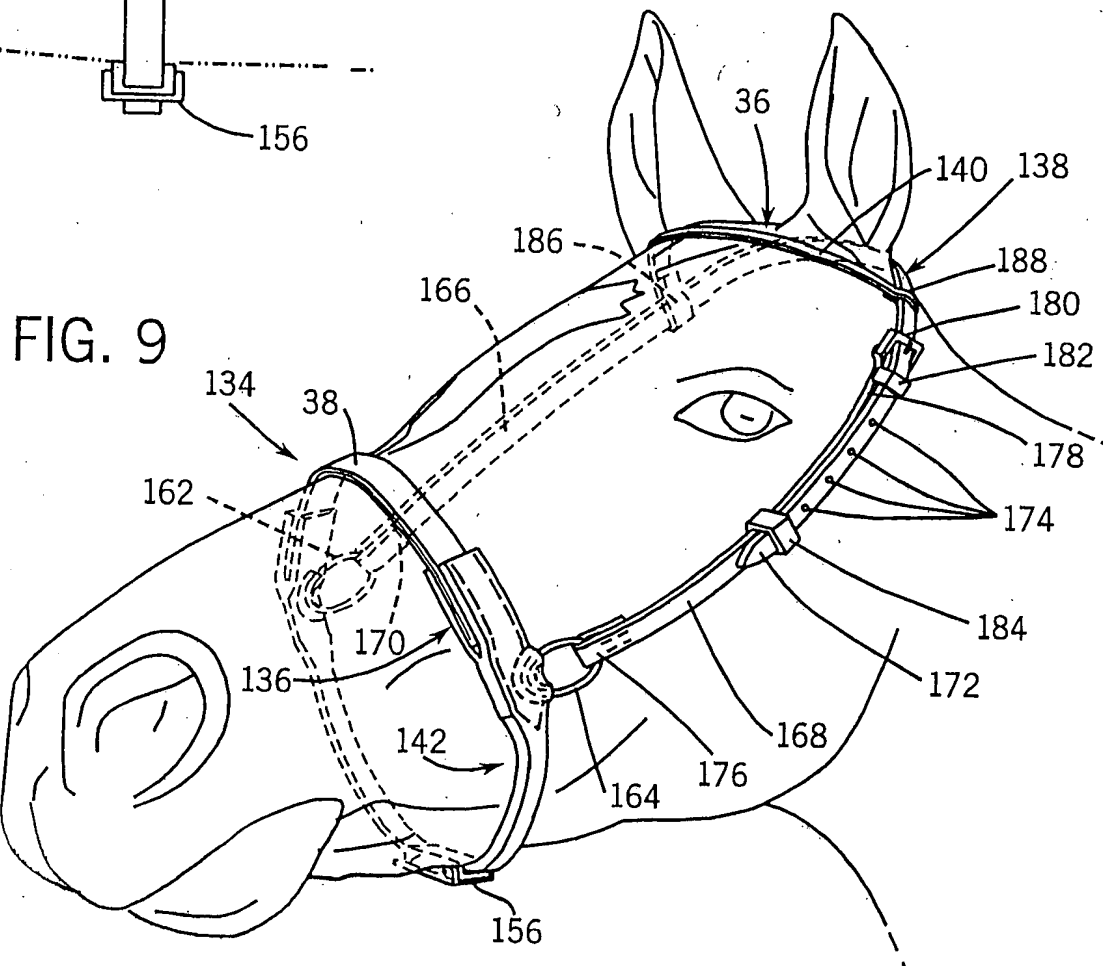
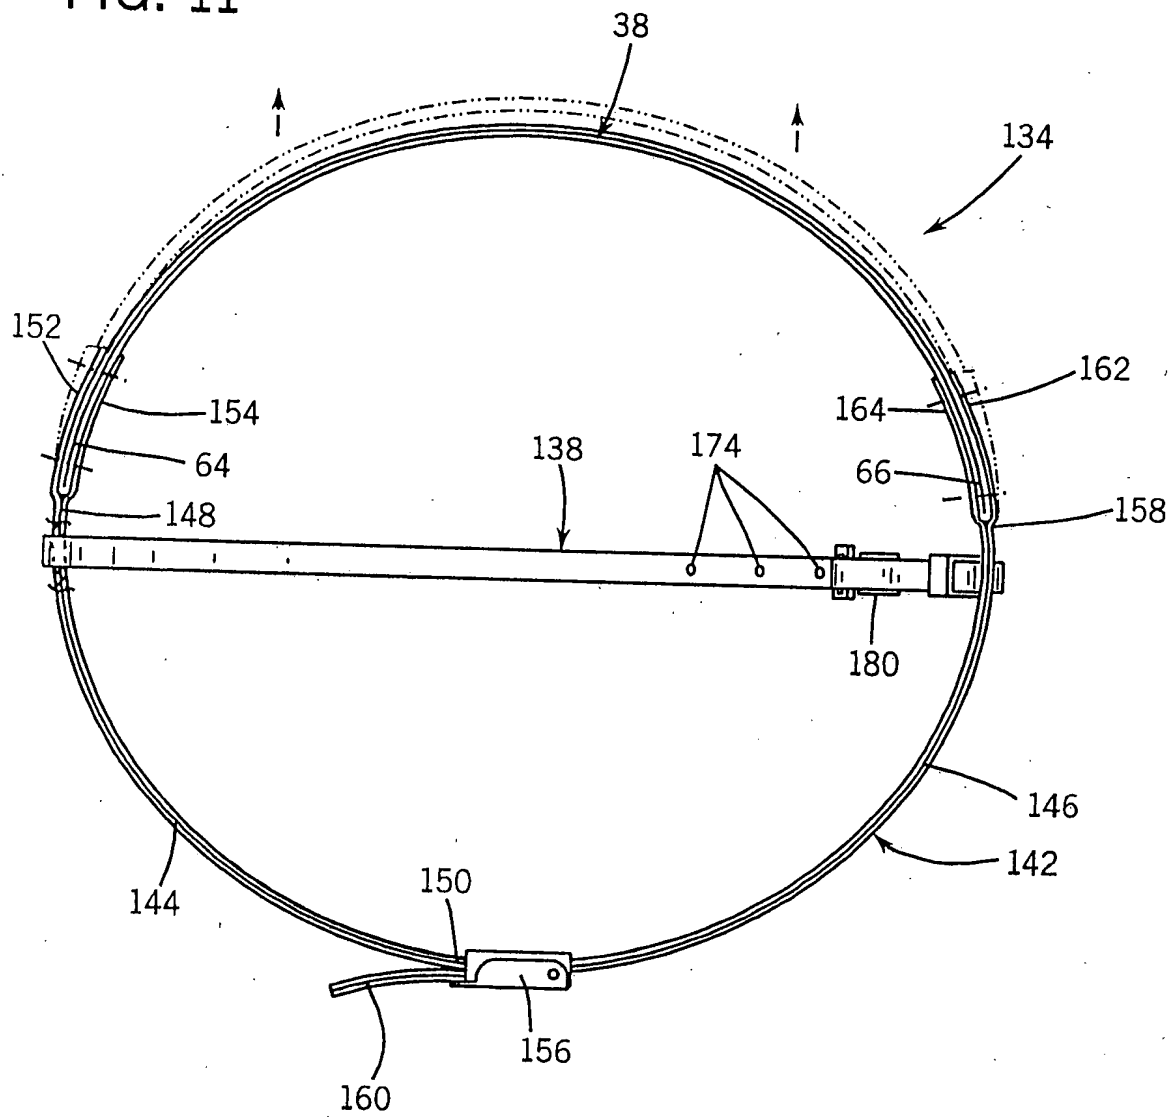


FIG. 11



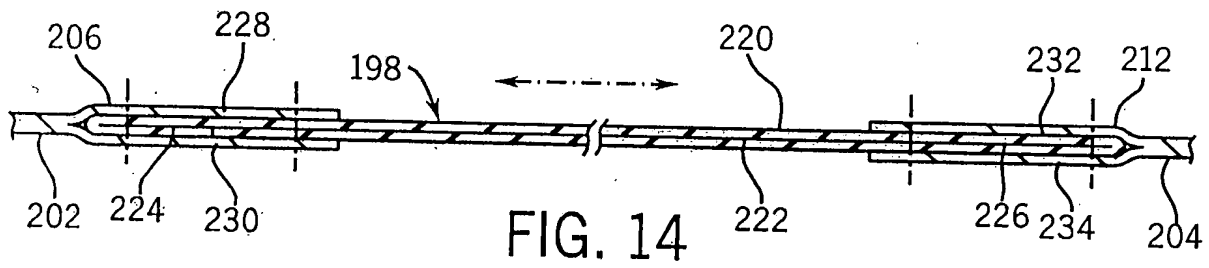
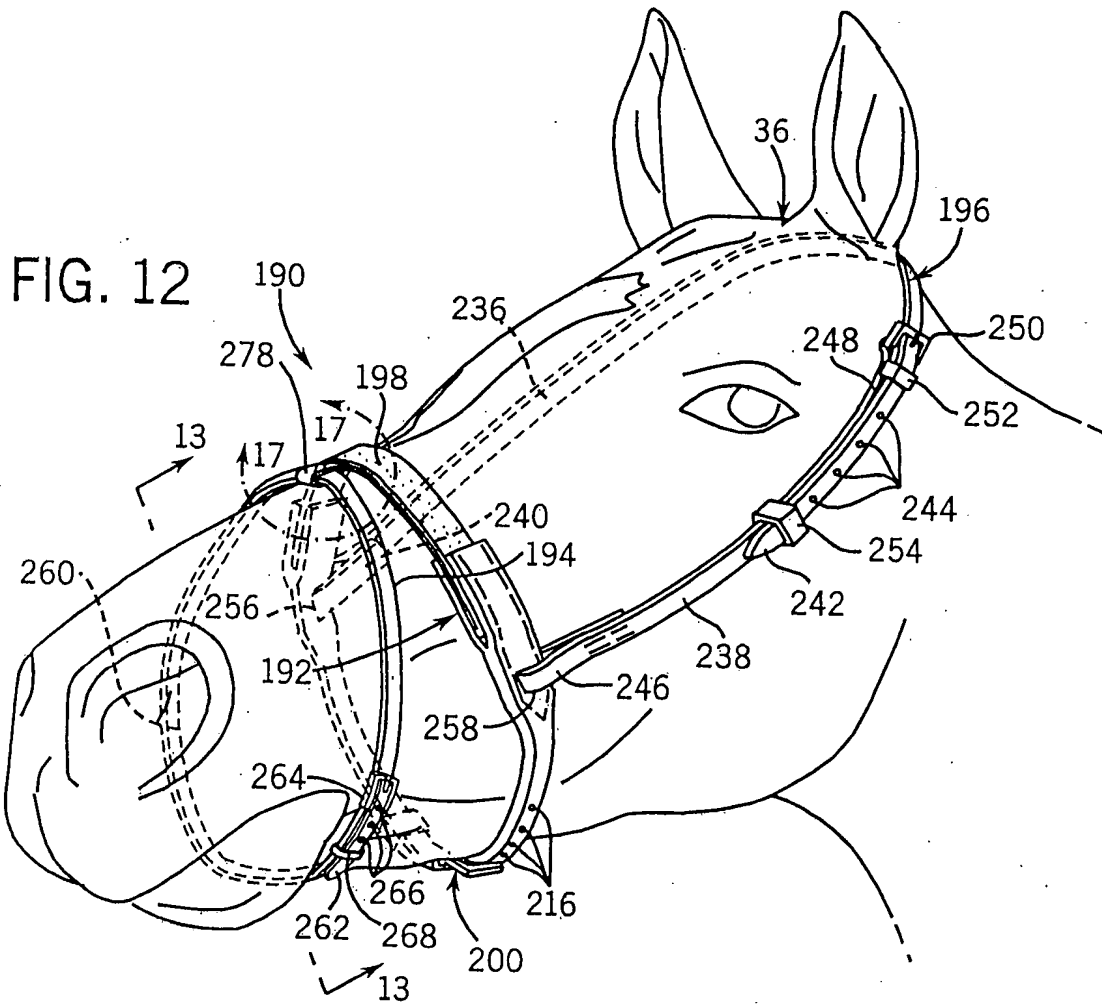


FIG. 13

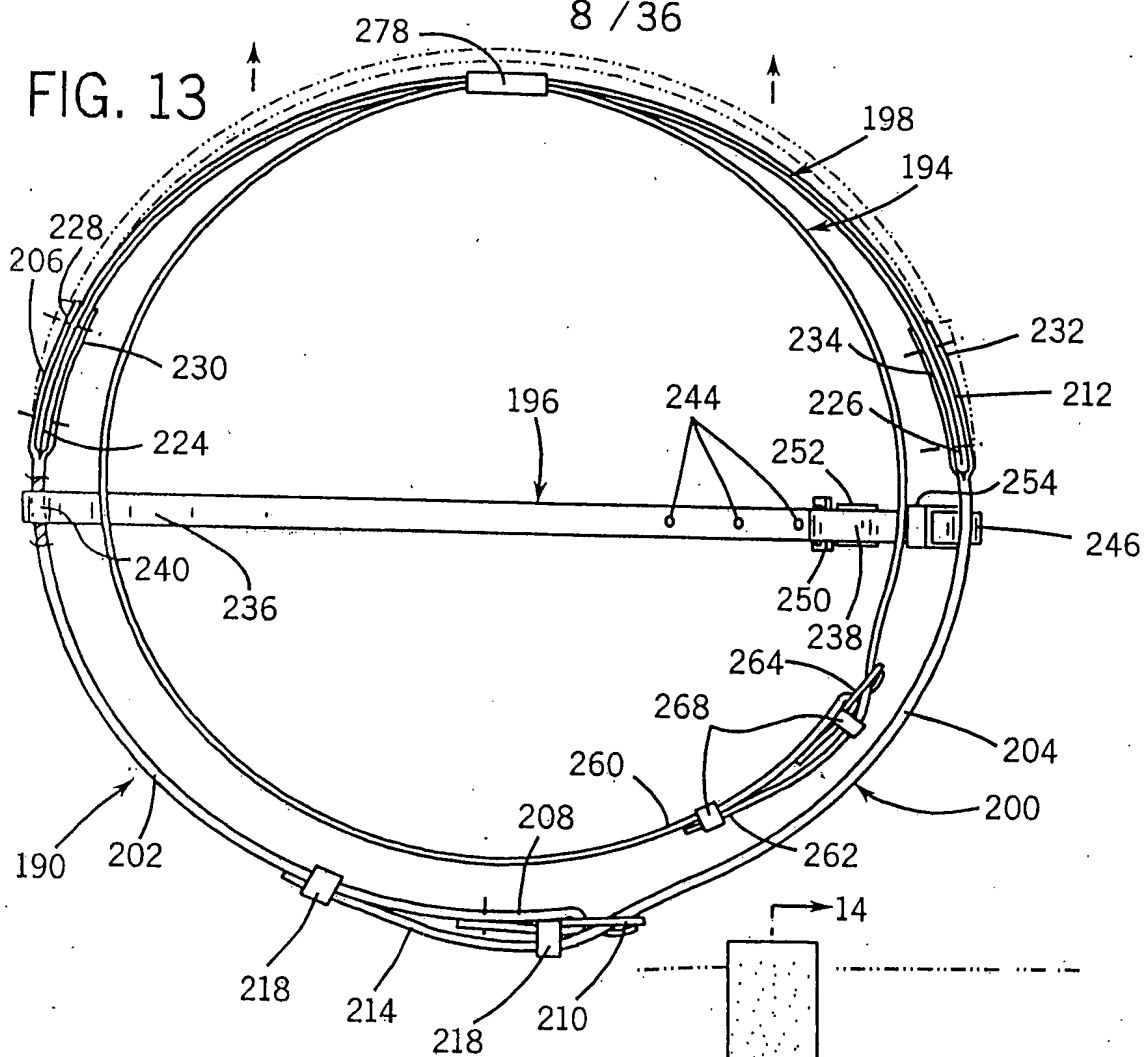


FIG. 15

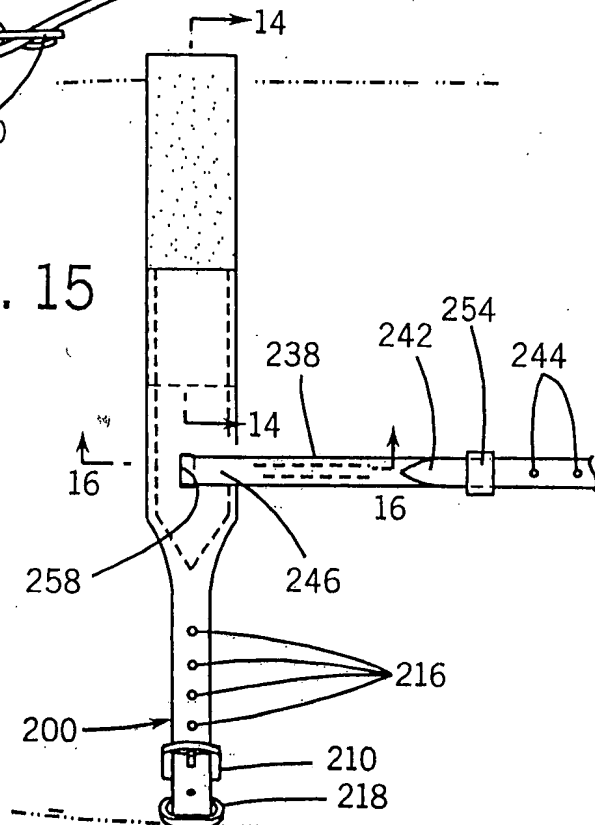


FIG. 16

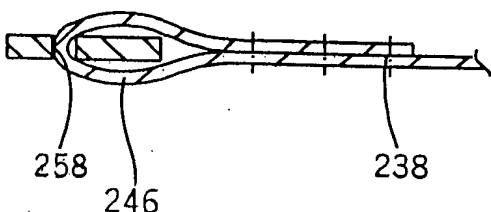




FIG. 17

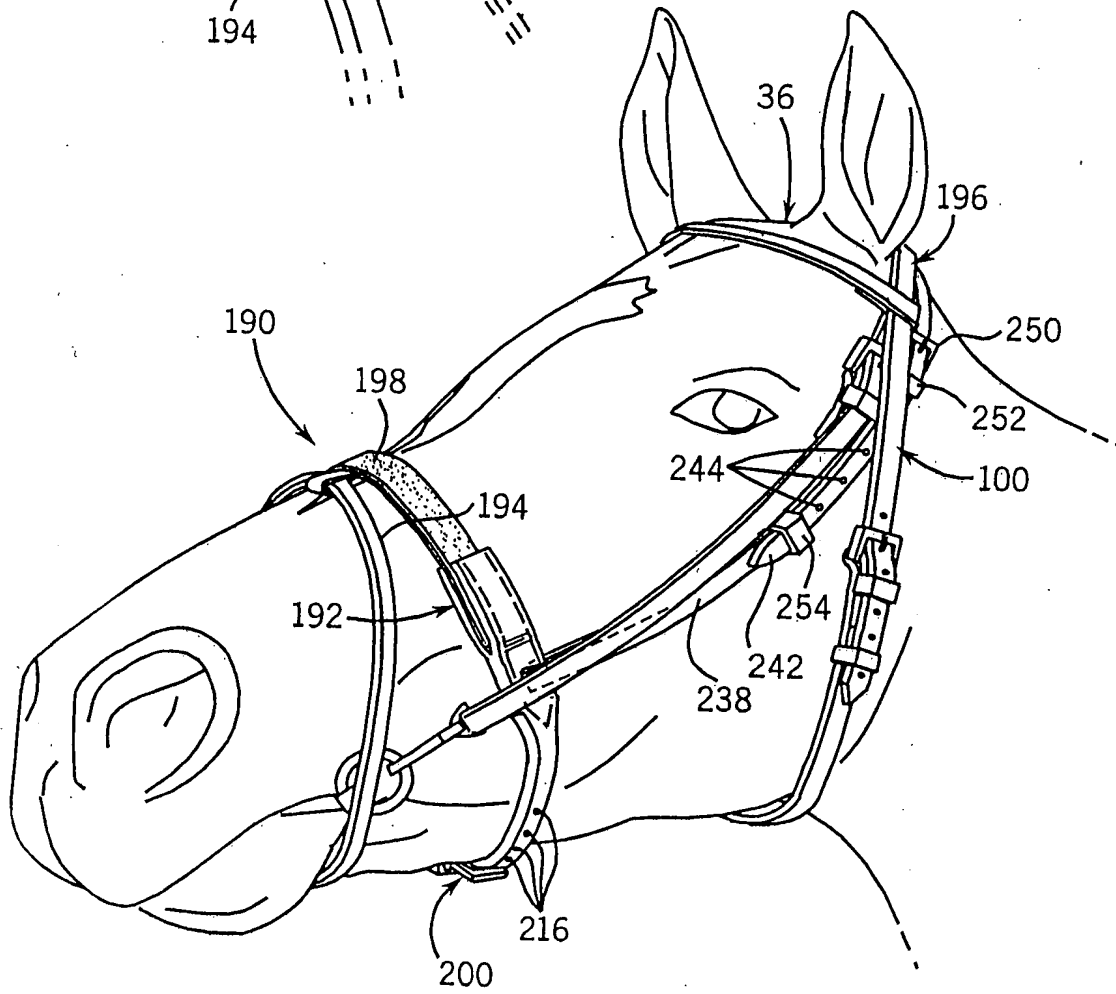
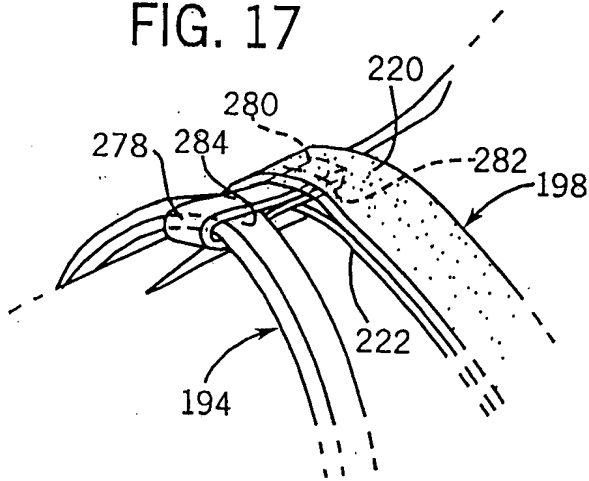
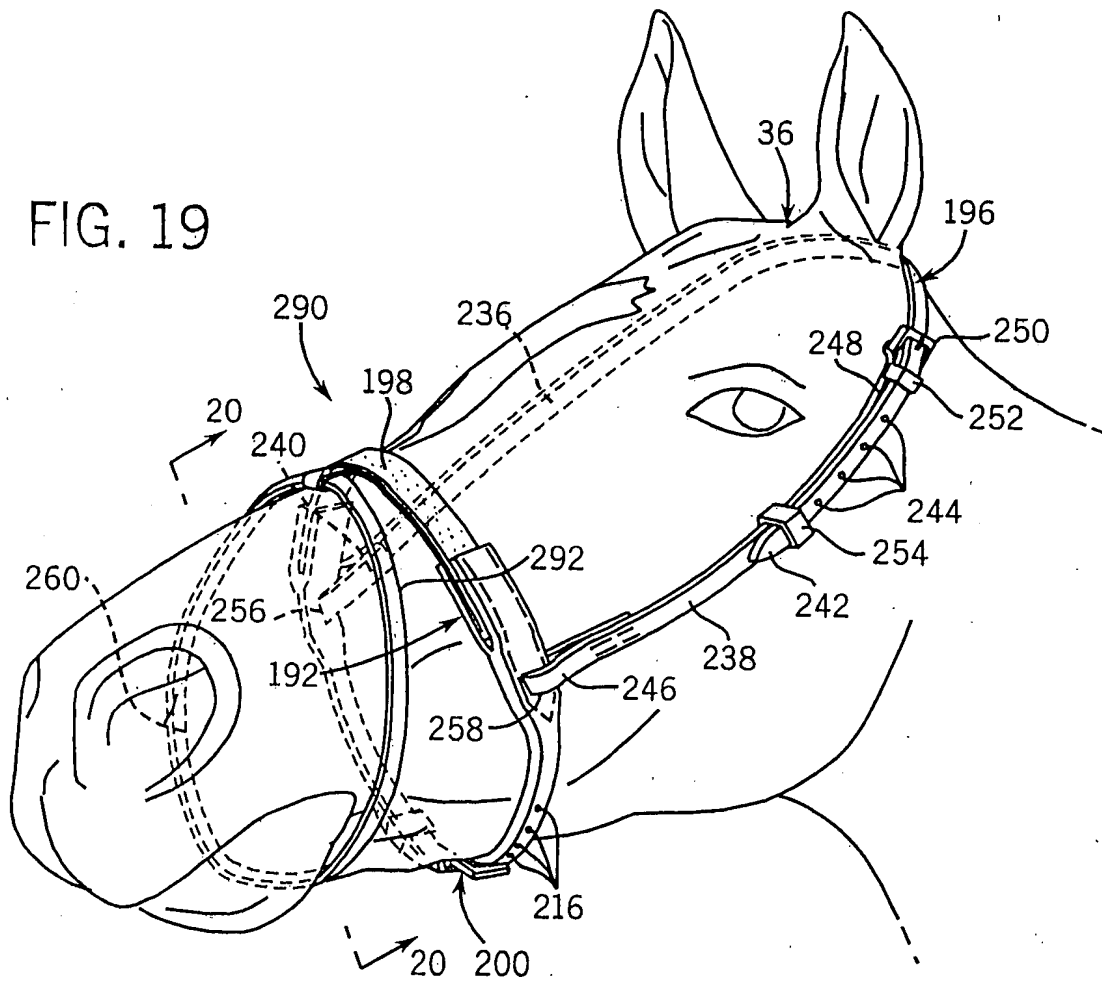
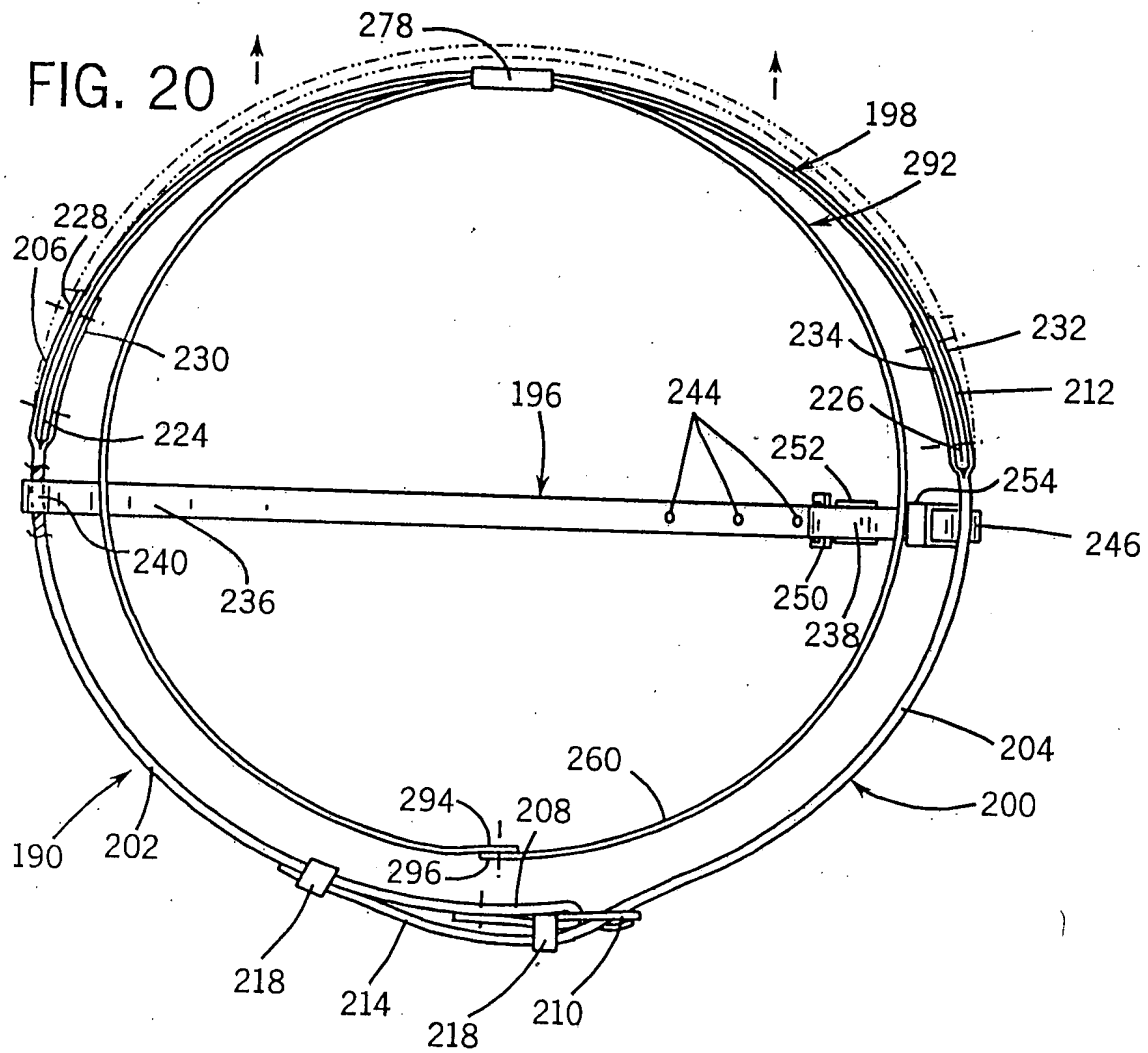


FIG. 18

FIG. 19





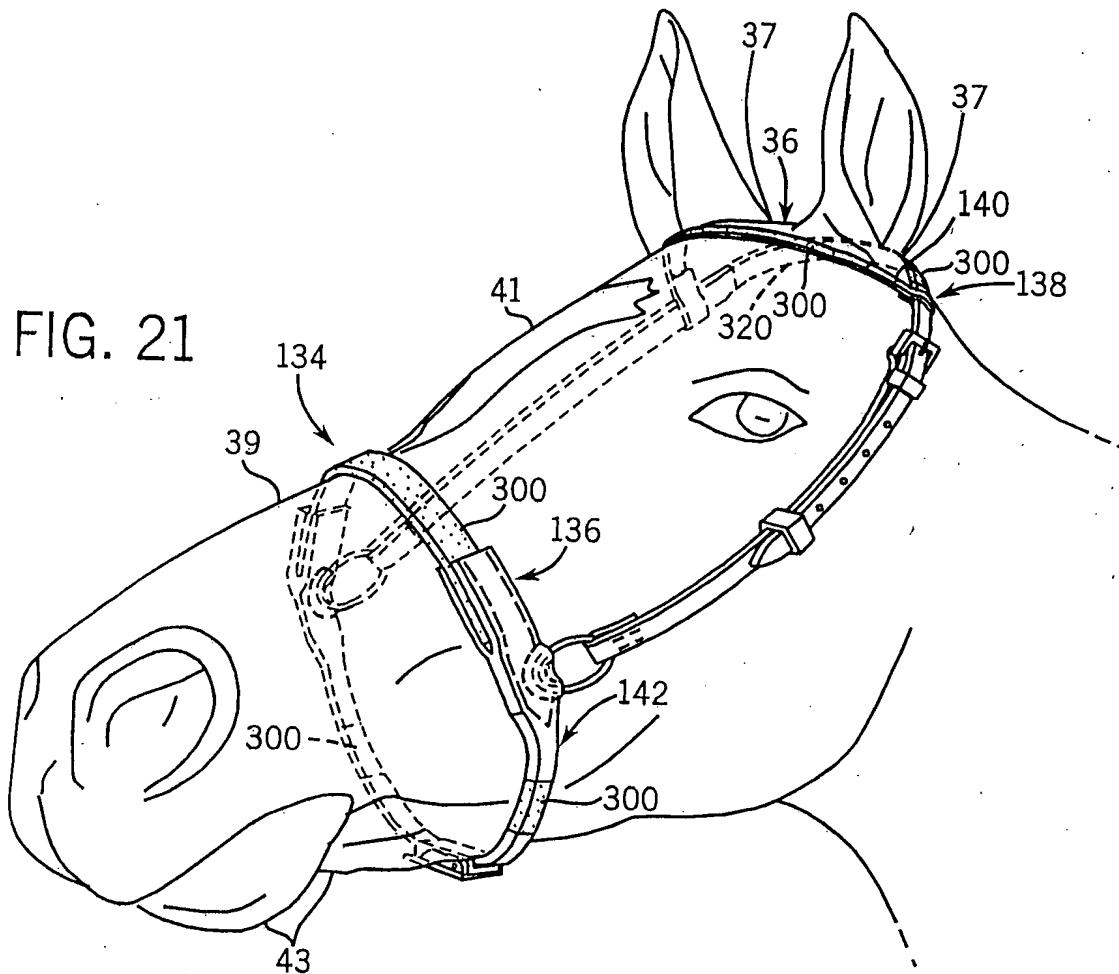
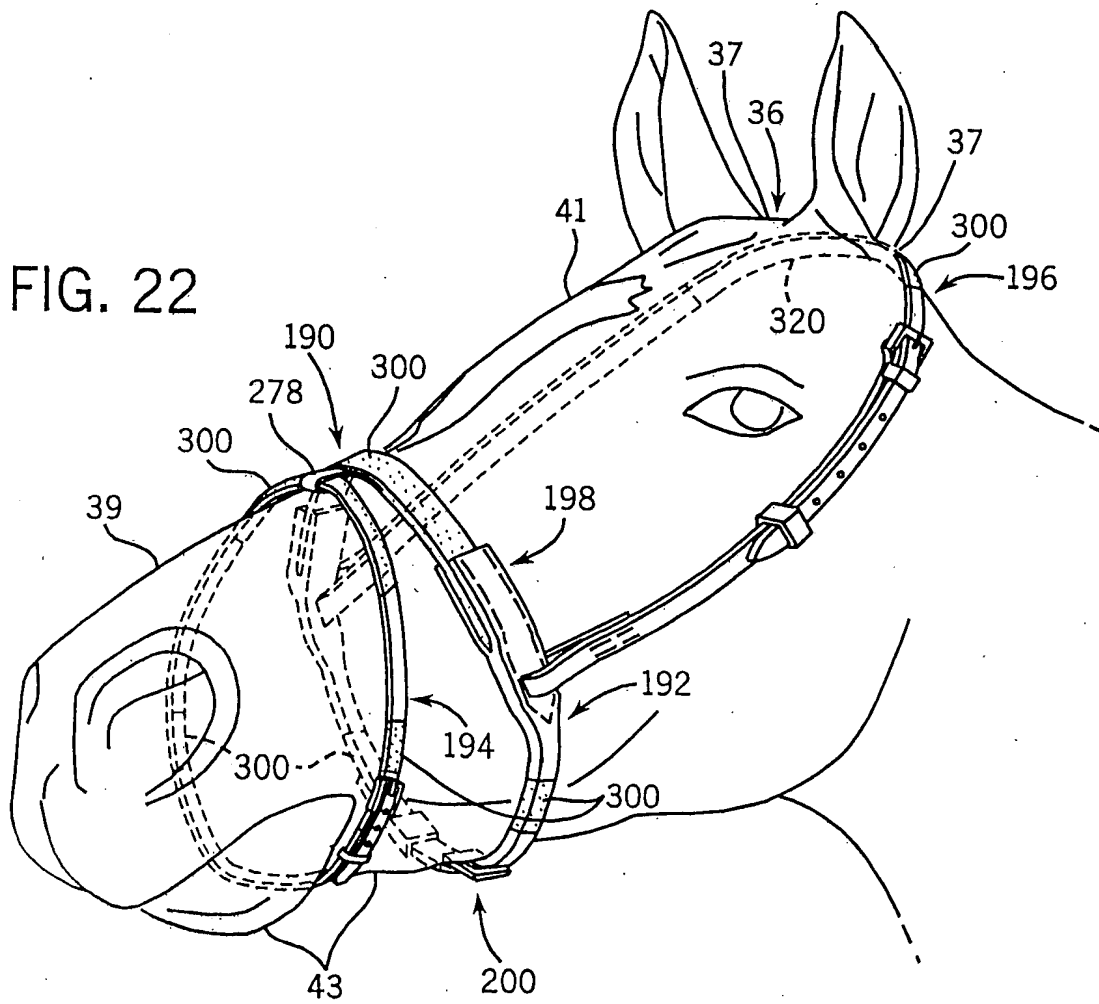


FIG. 22



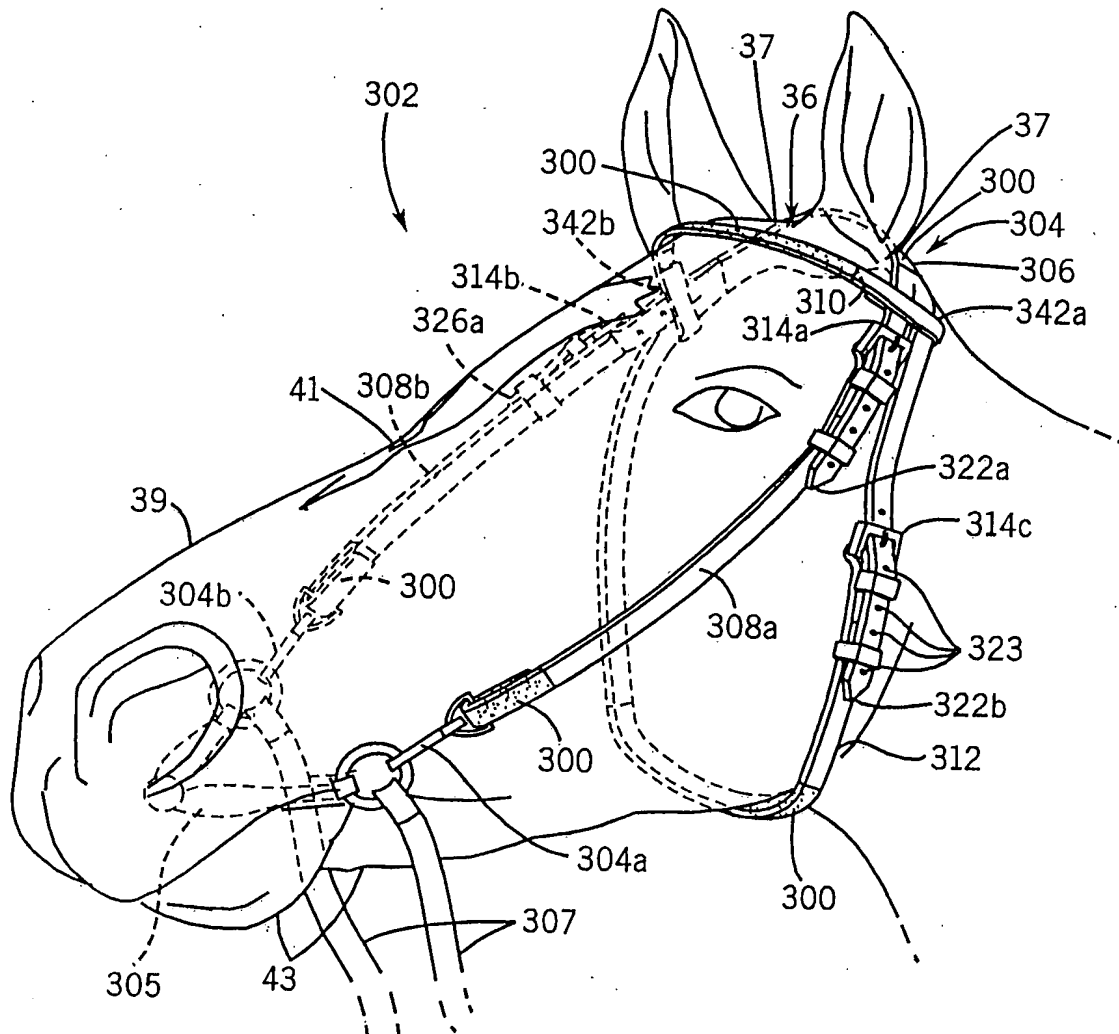


FIG. 23

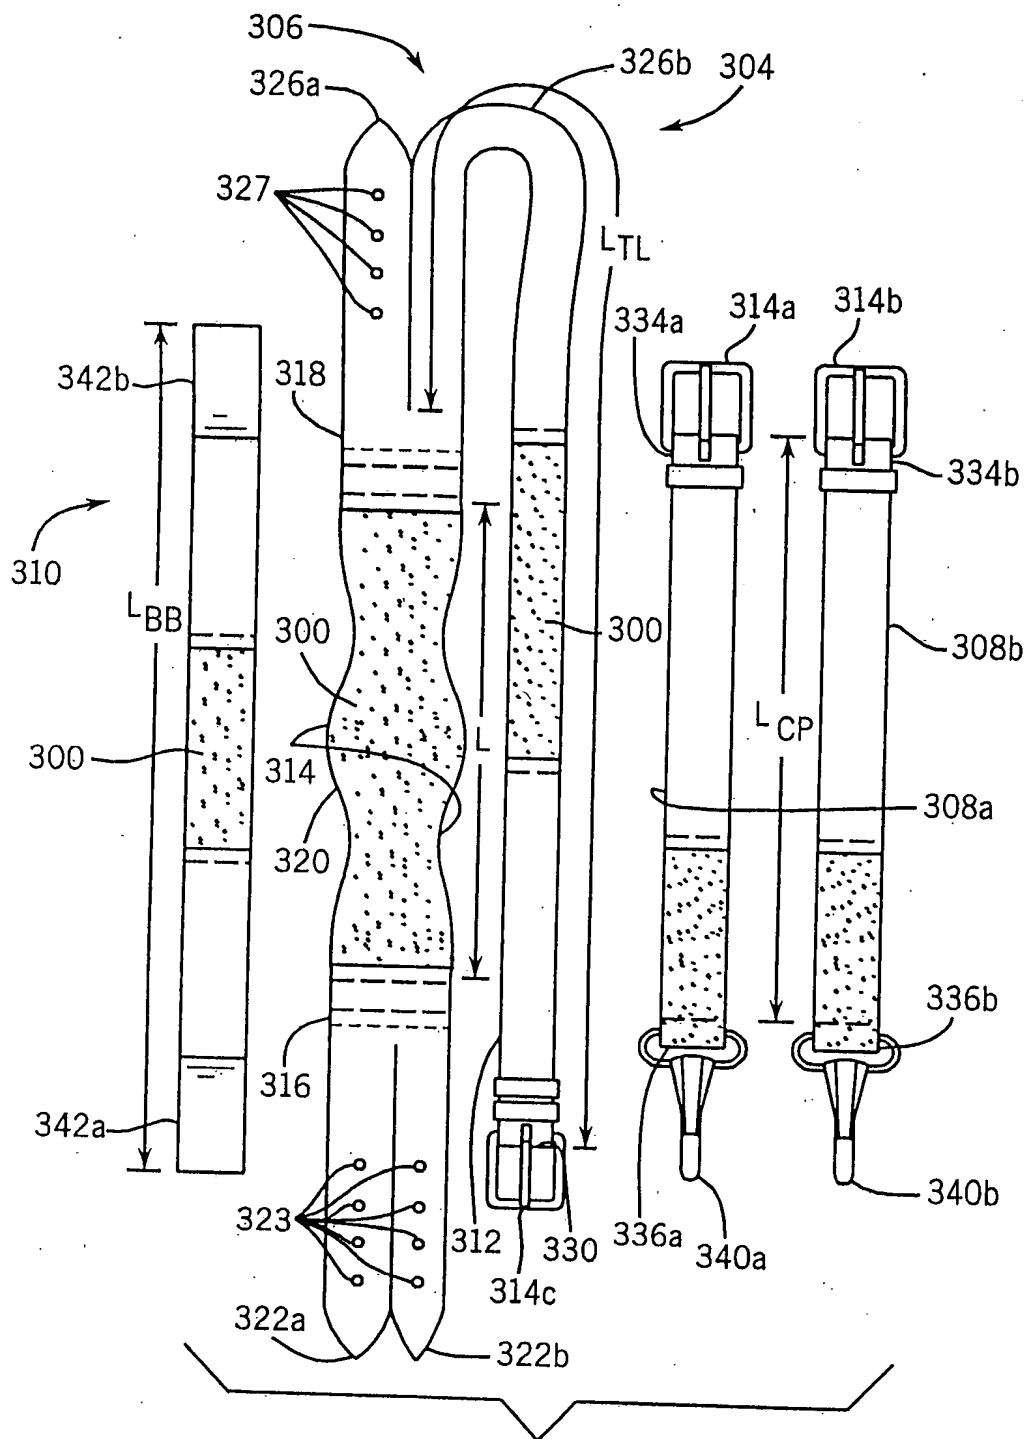
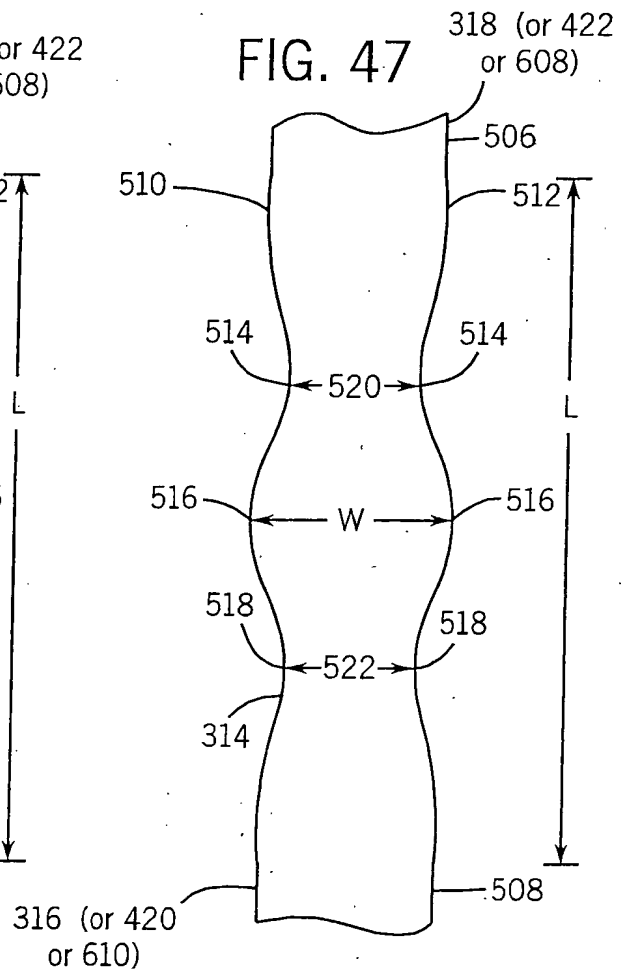
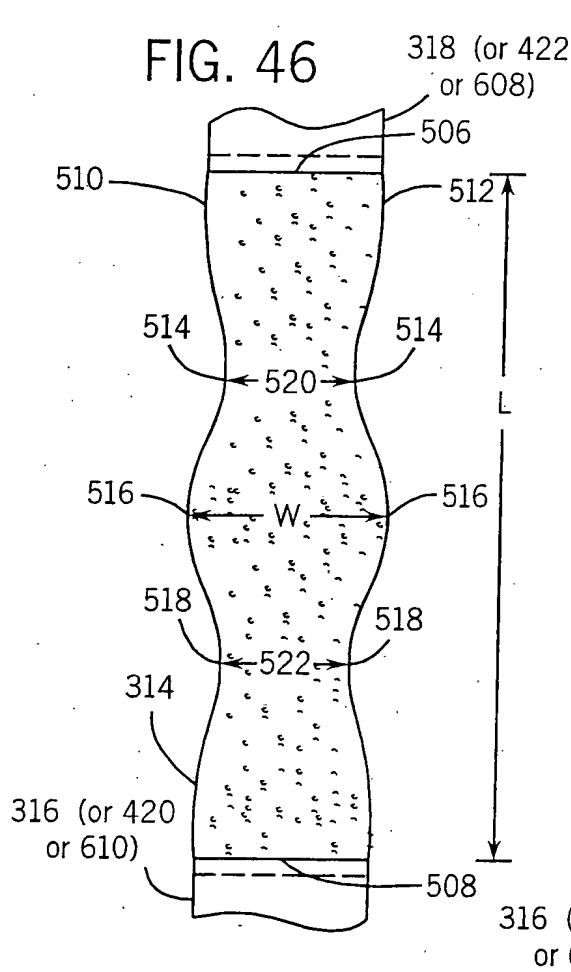
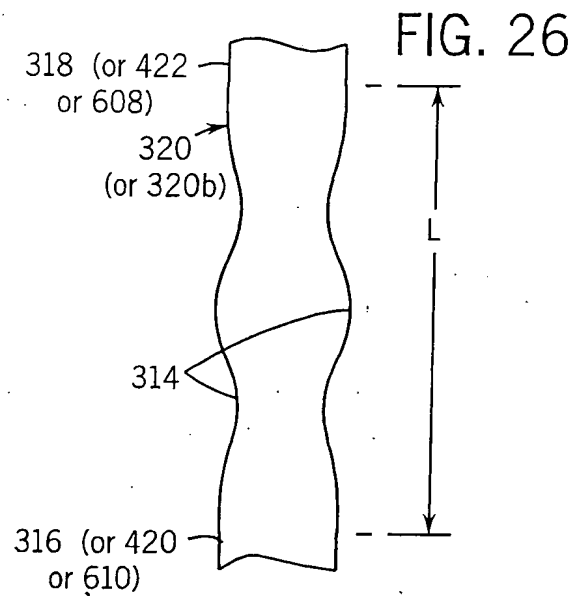
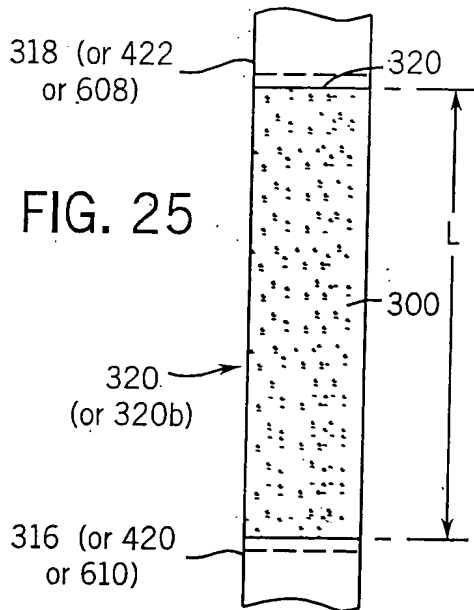
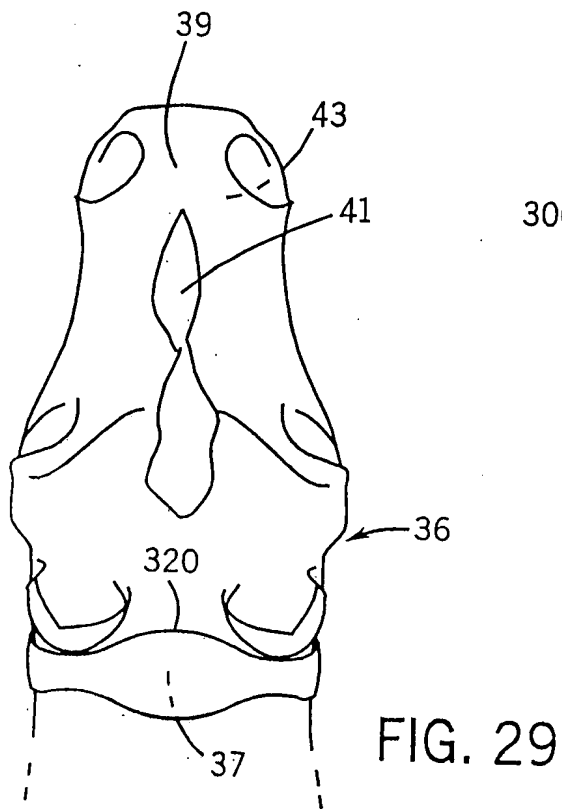
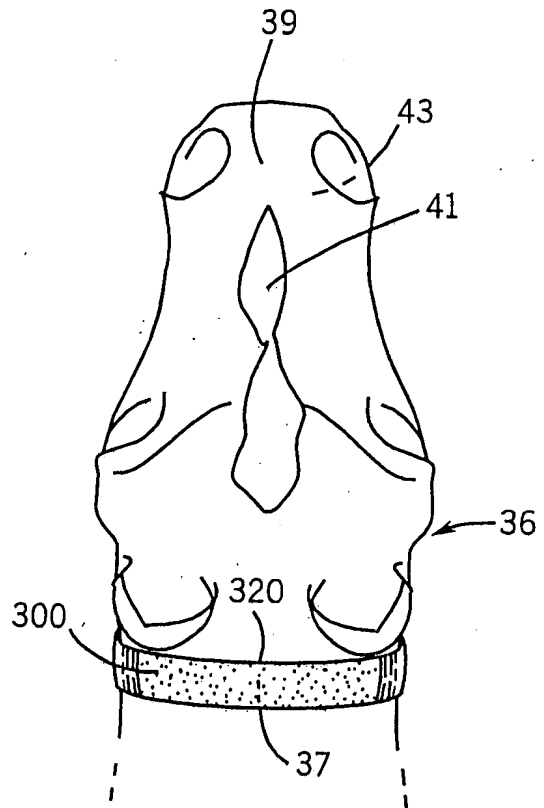
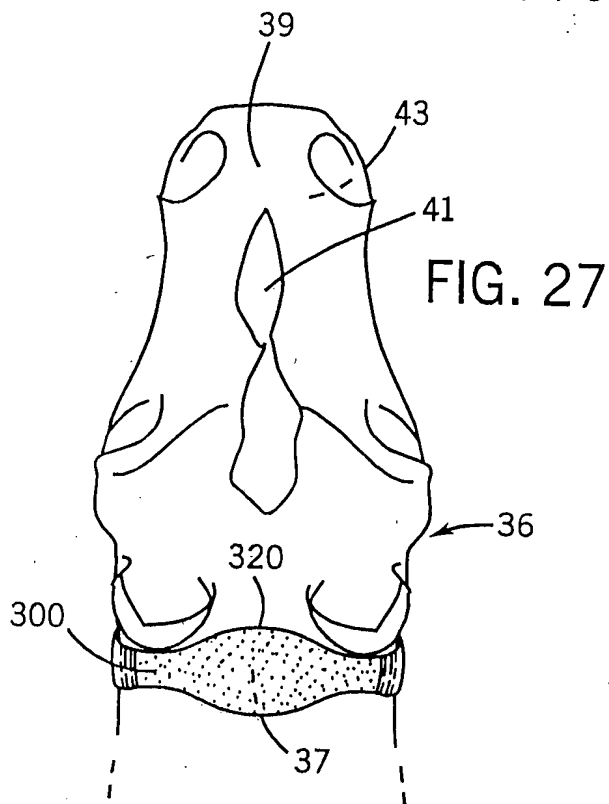


FIG. 24







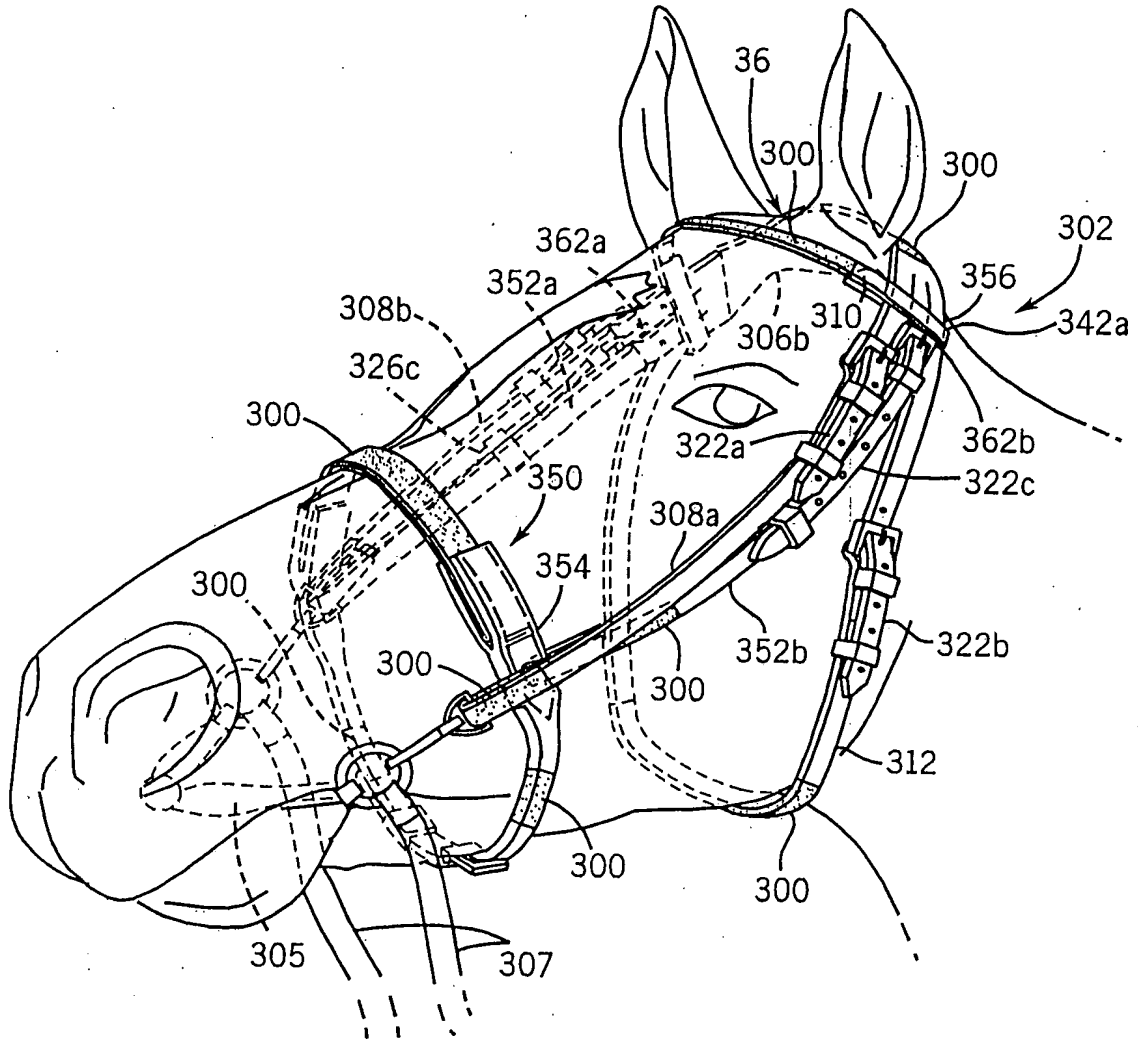
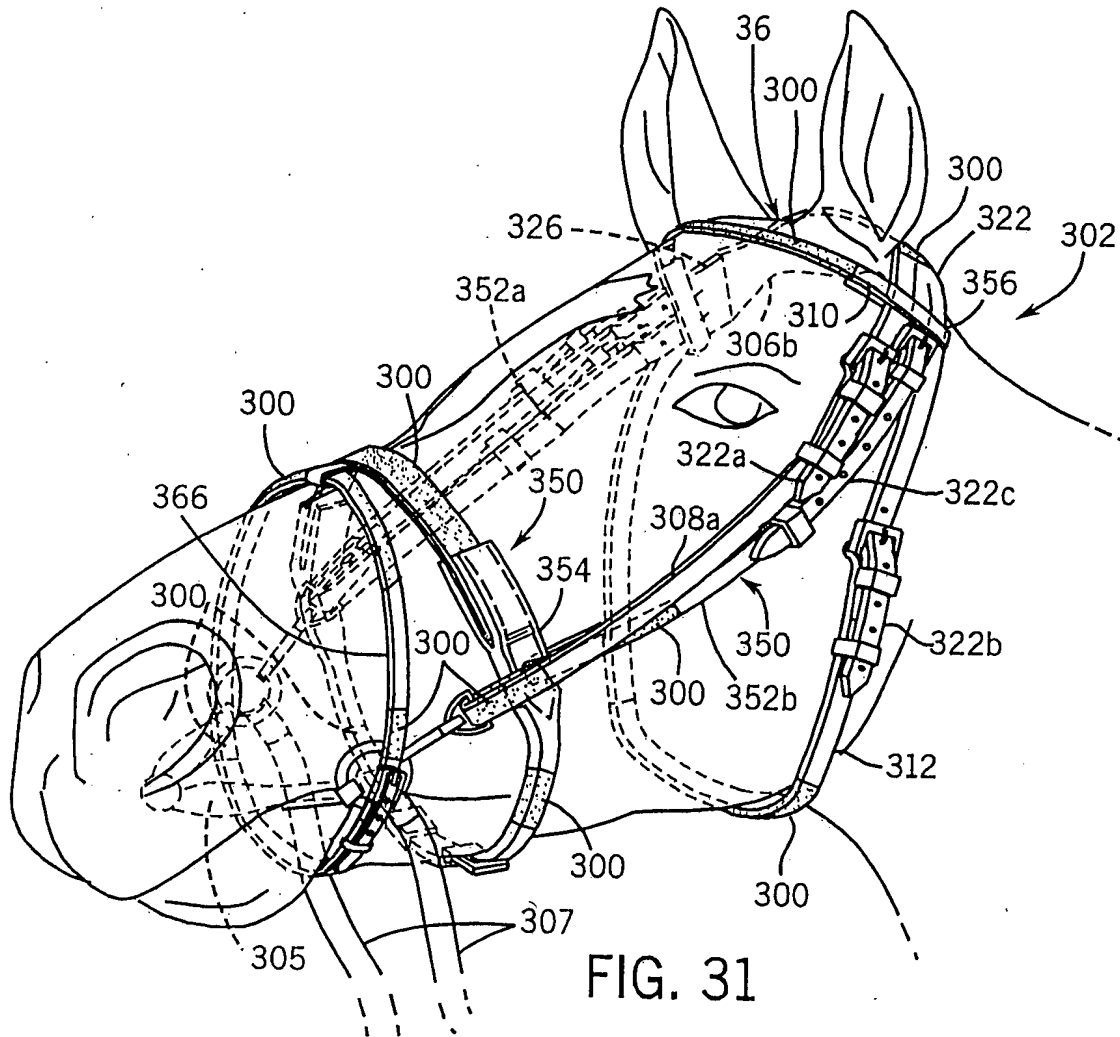


FIG. 30



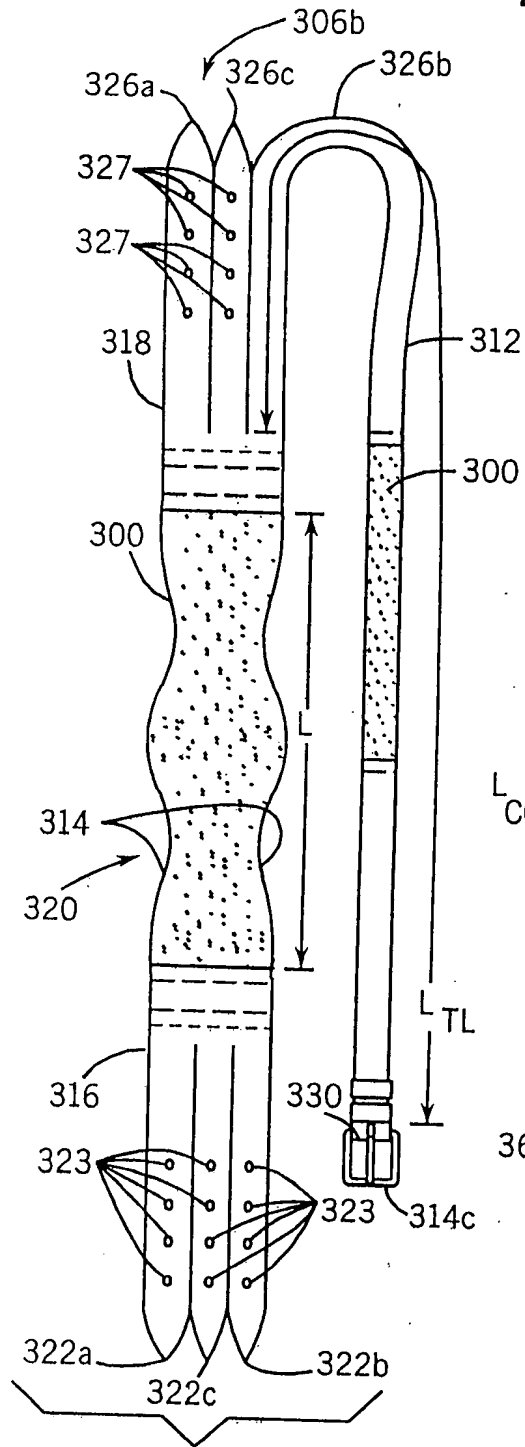


FIG. 32

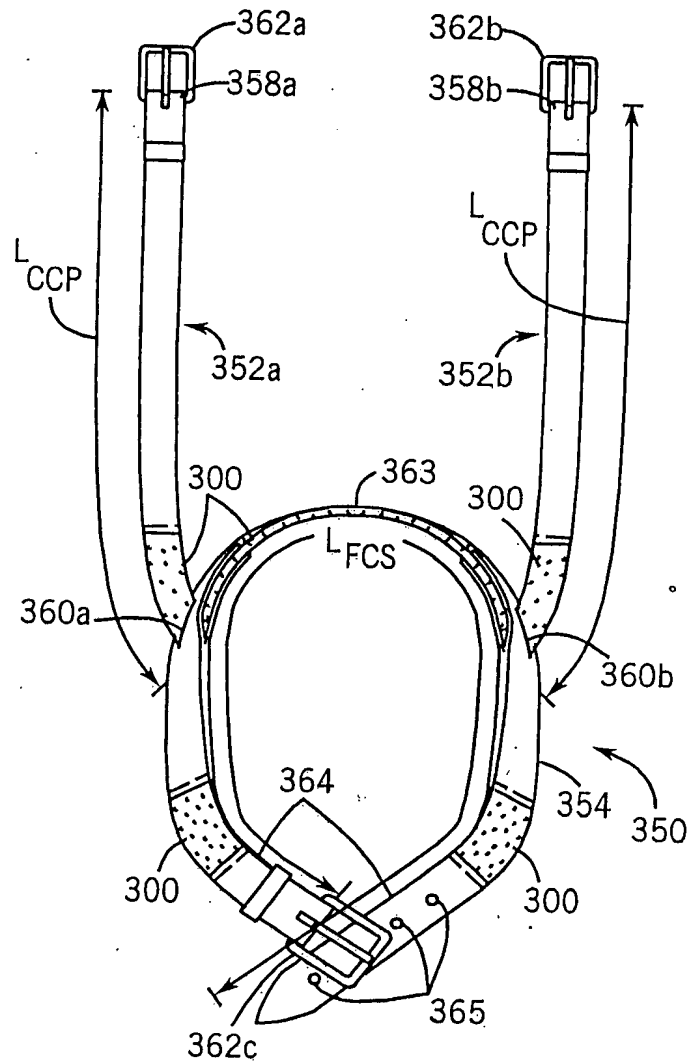
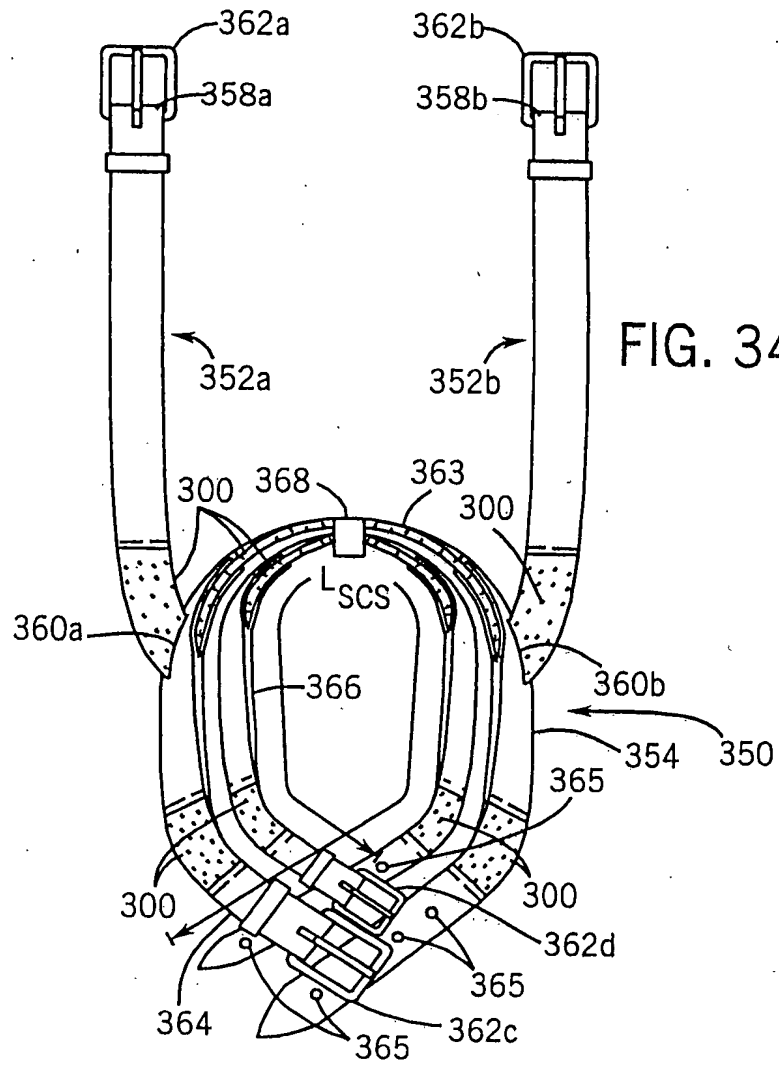
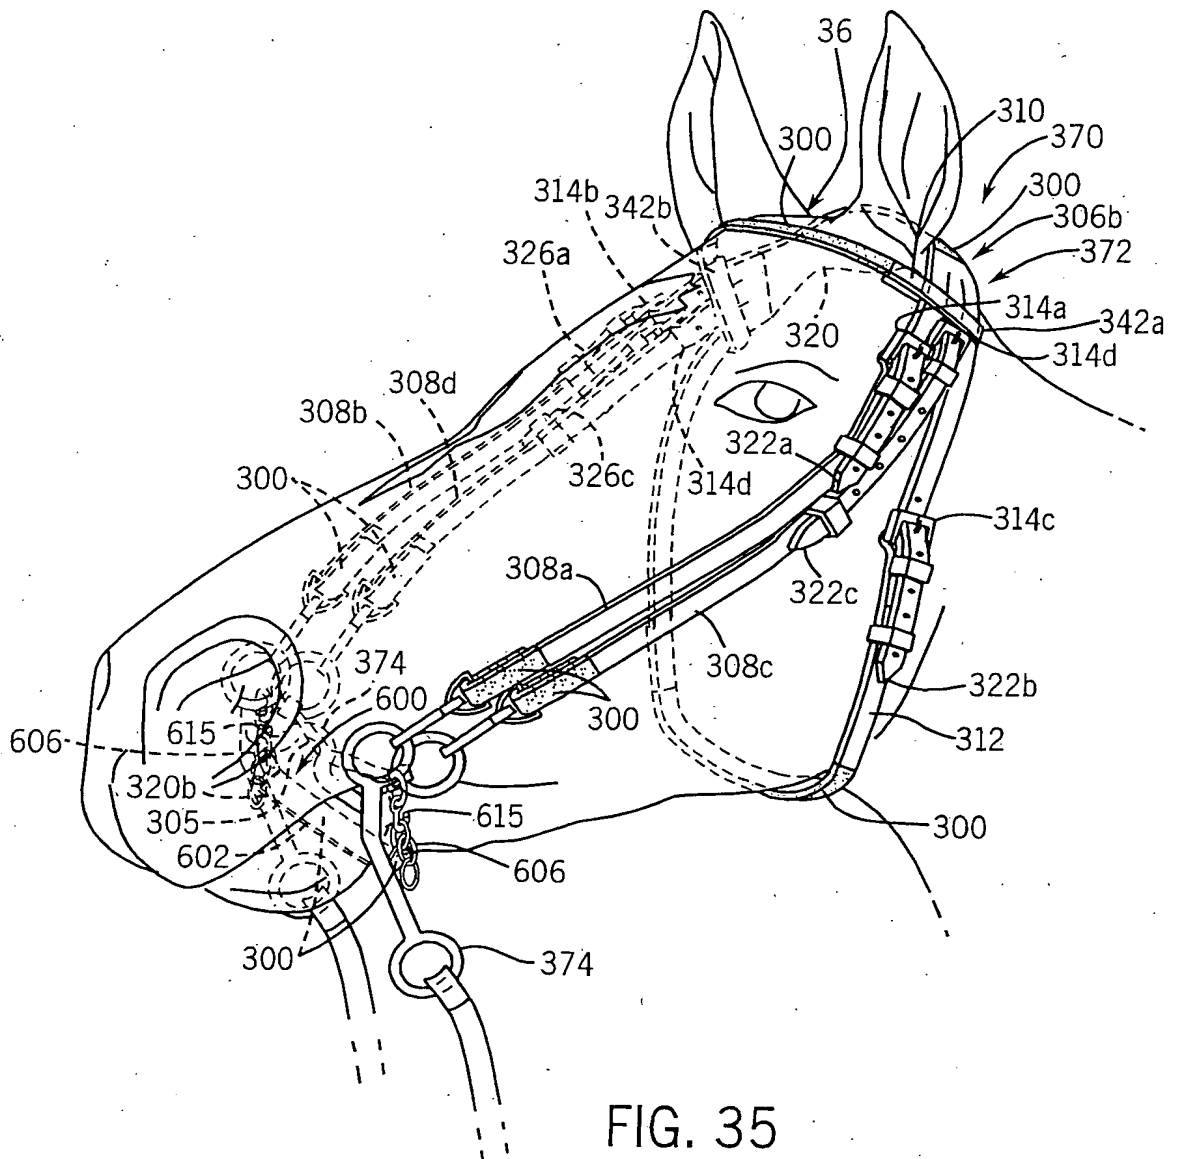


FIG. 33





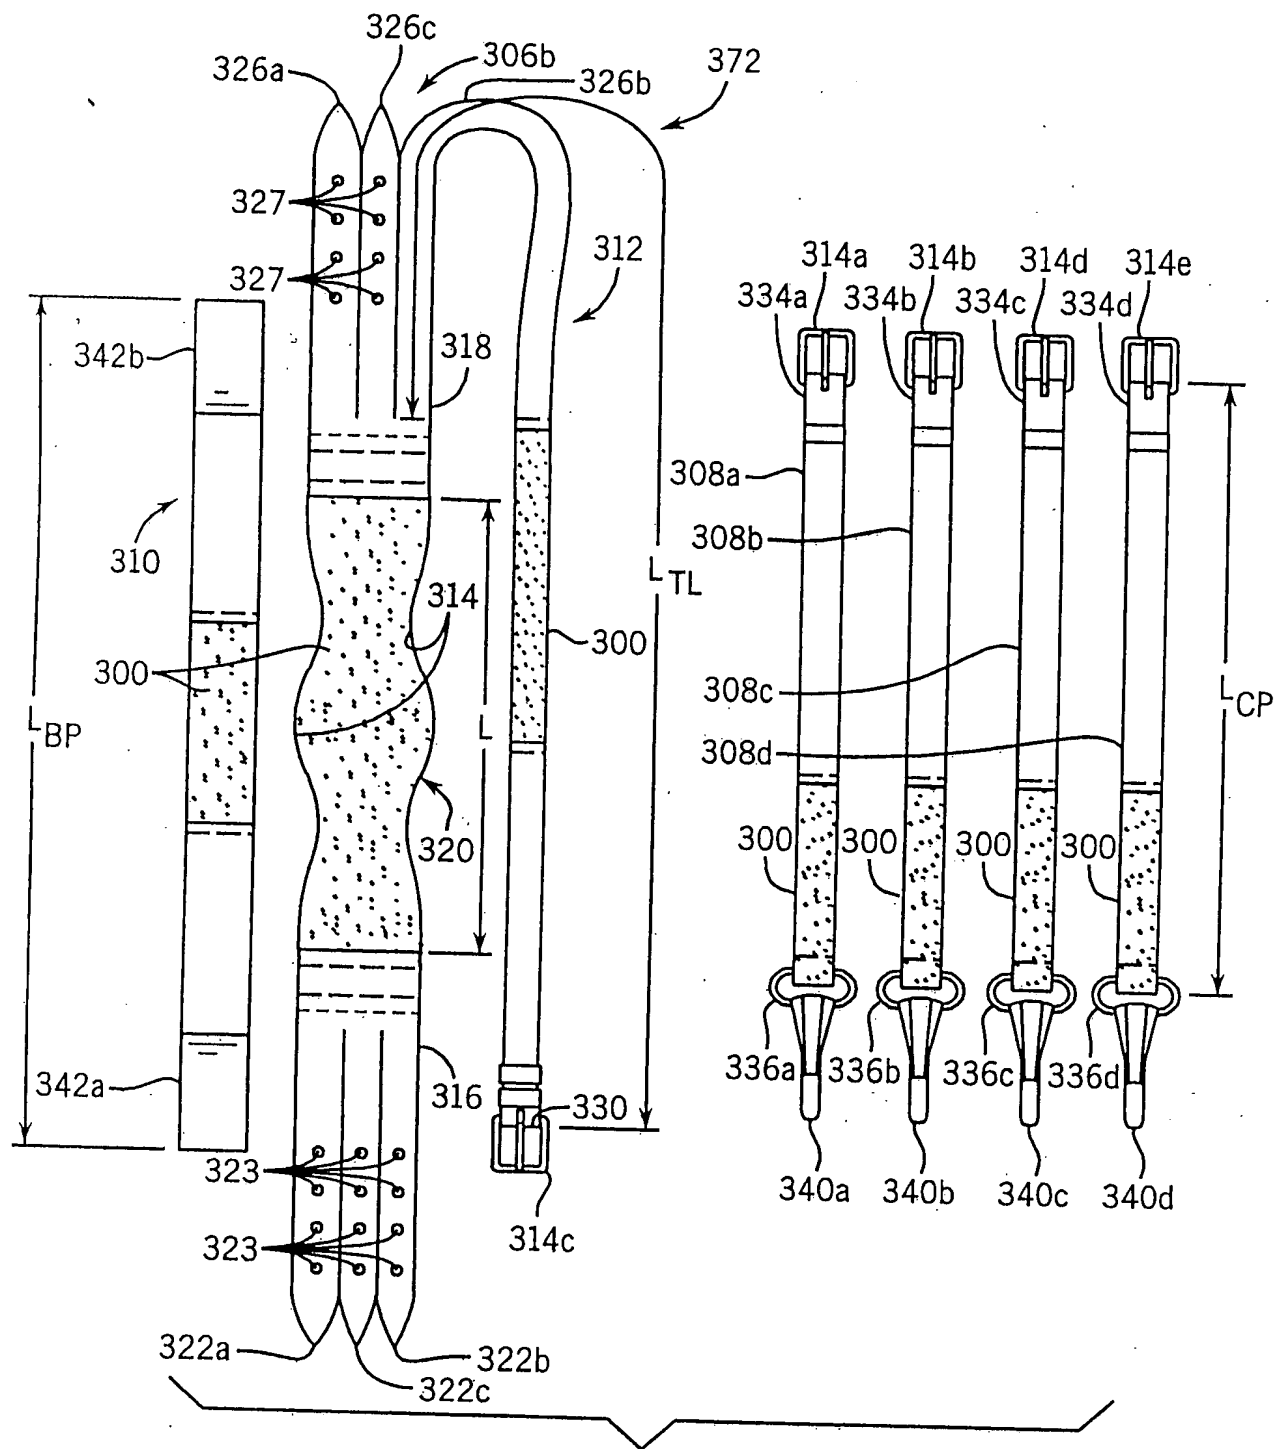
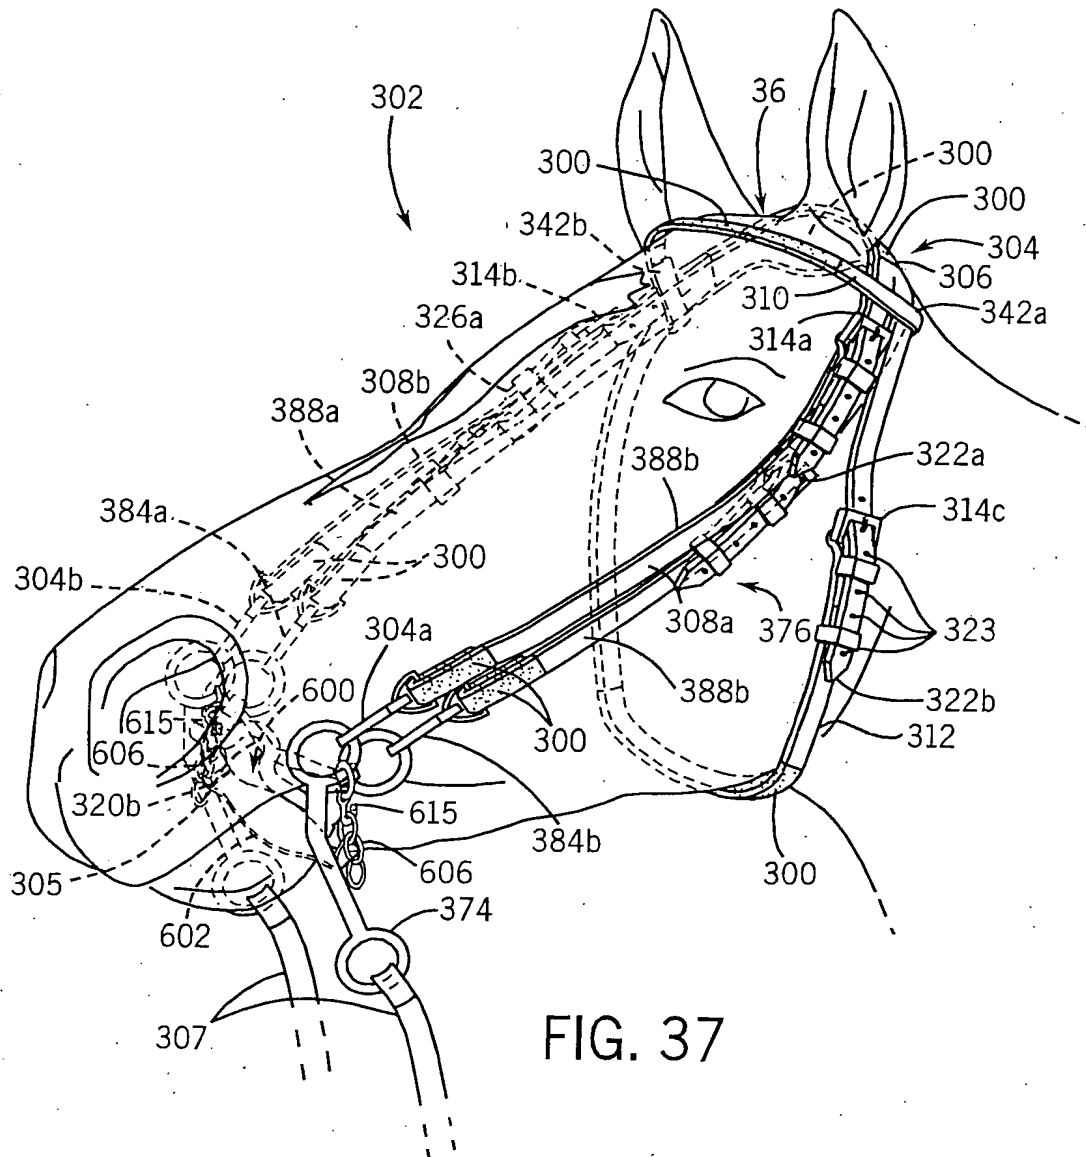


FIG. 36





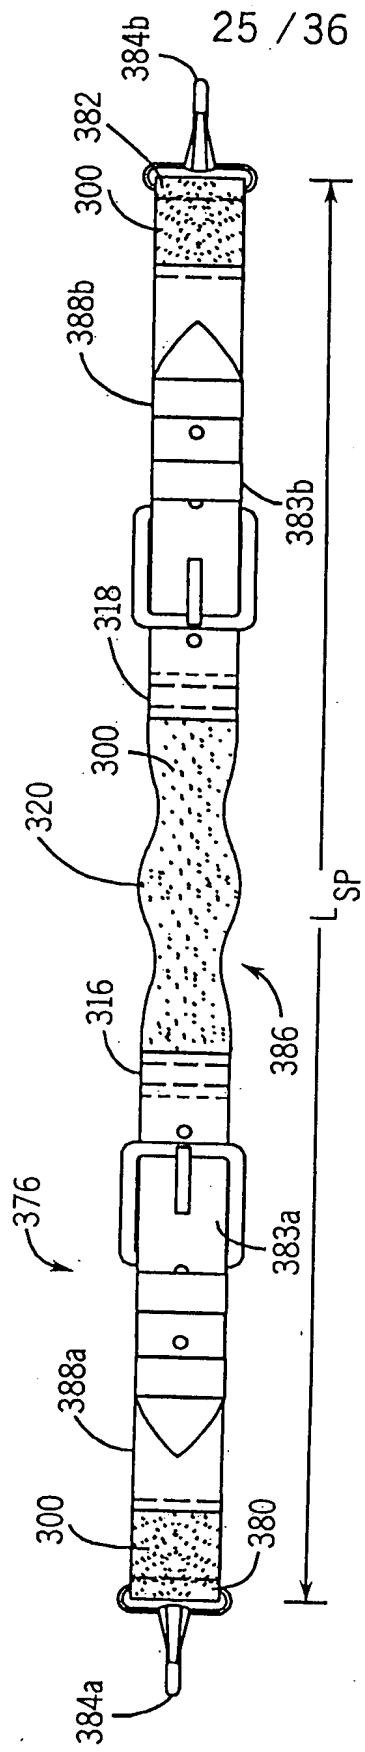
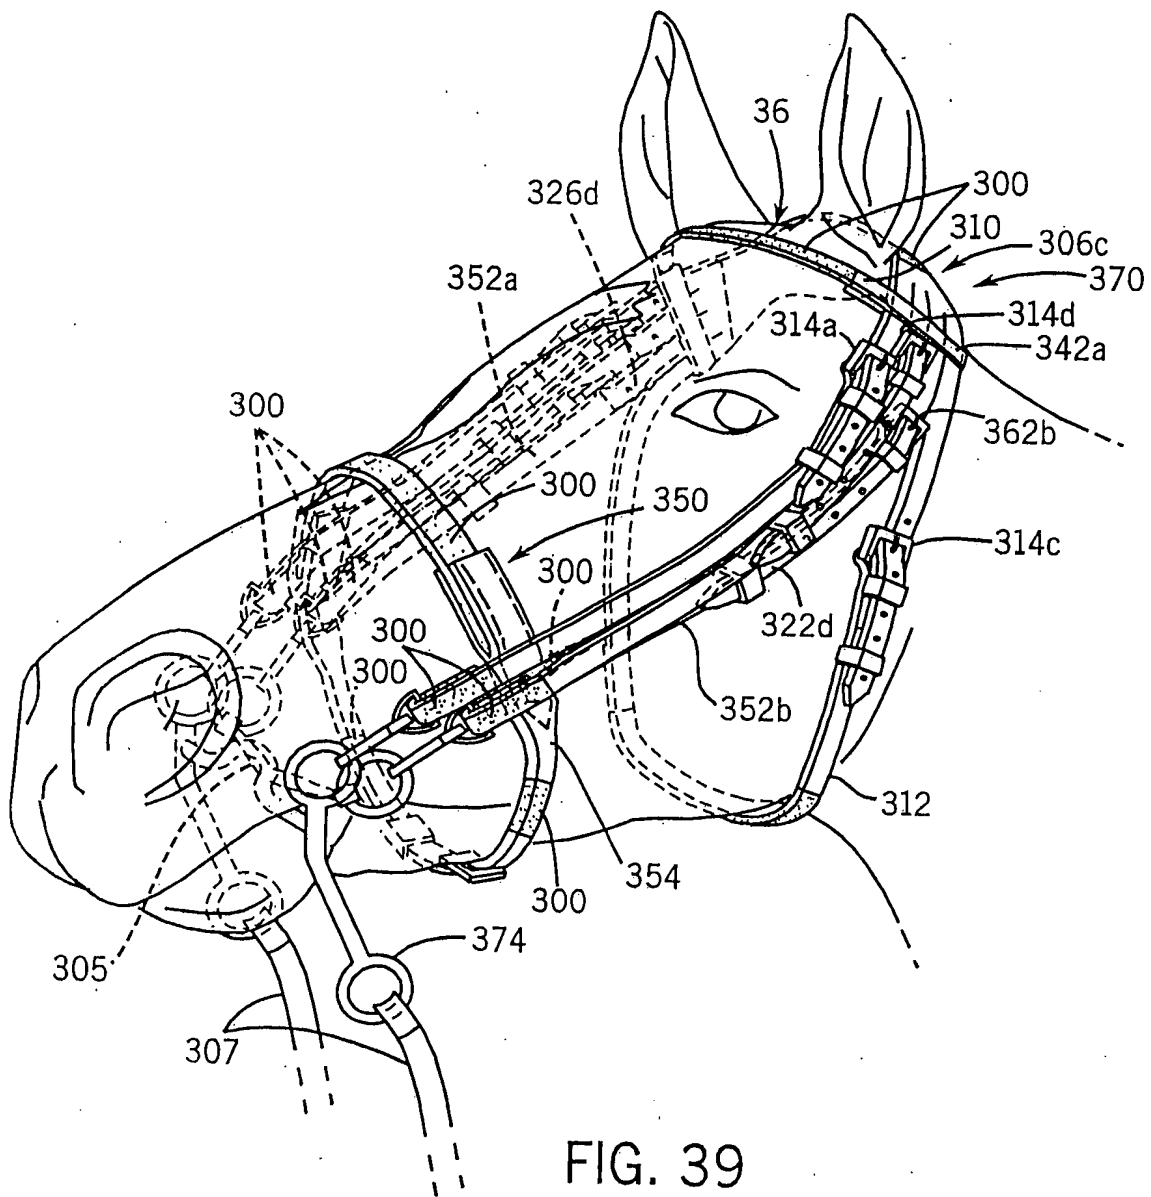


FIG. 38



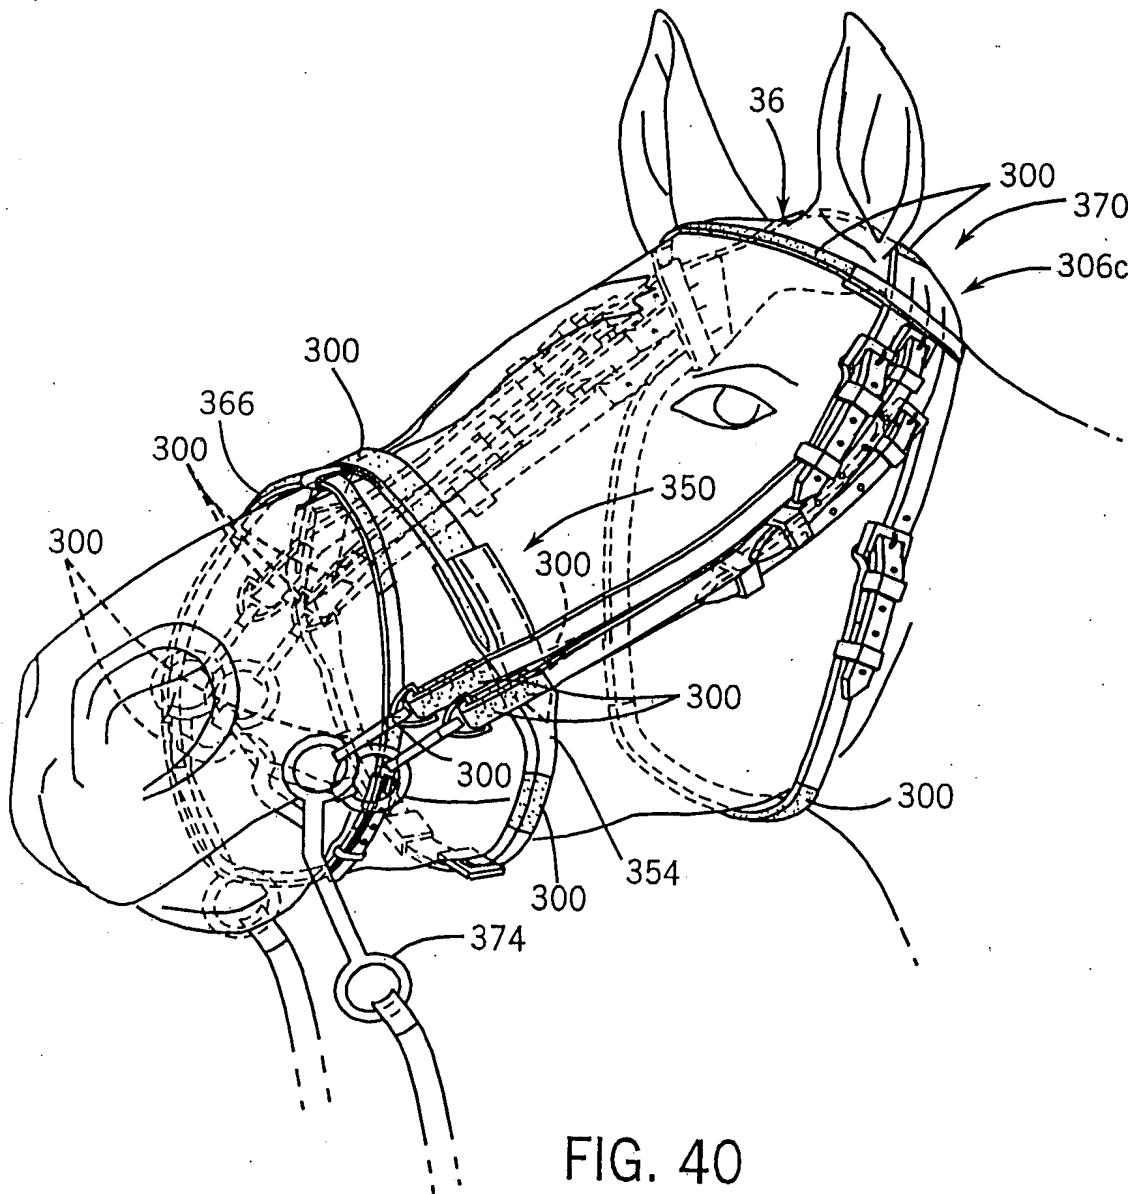


FIG. 40

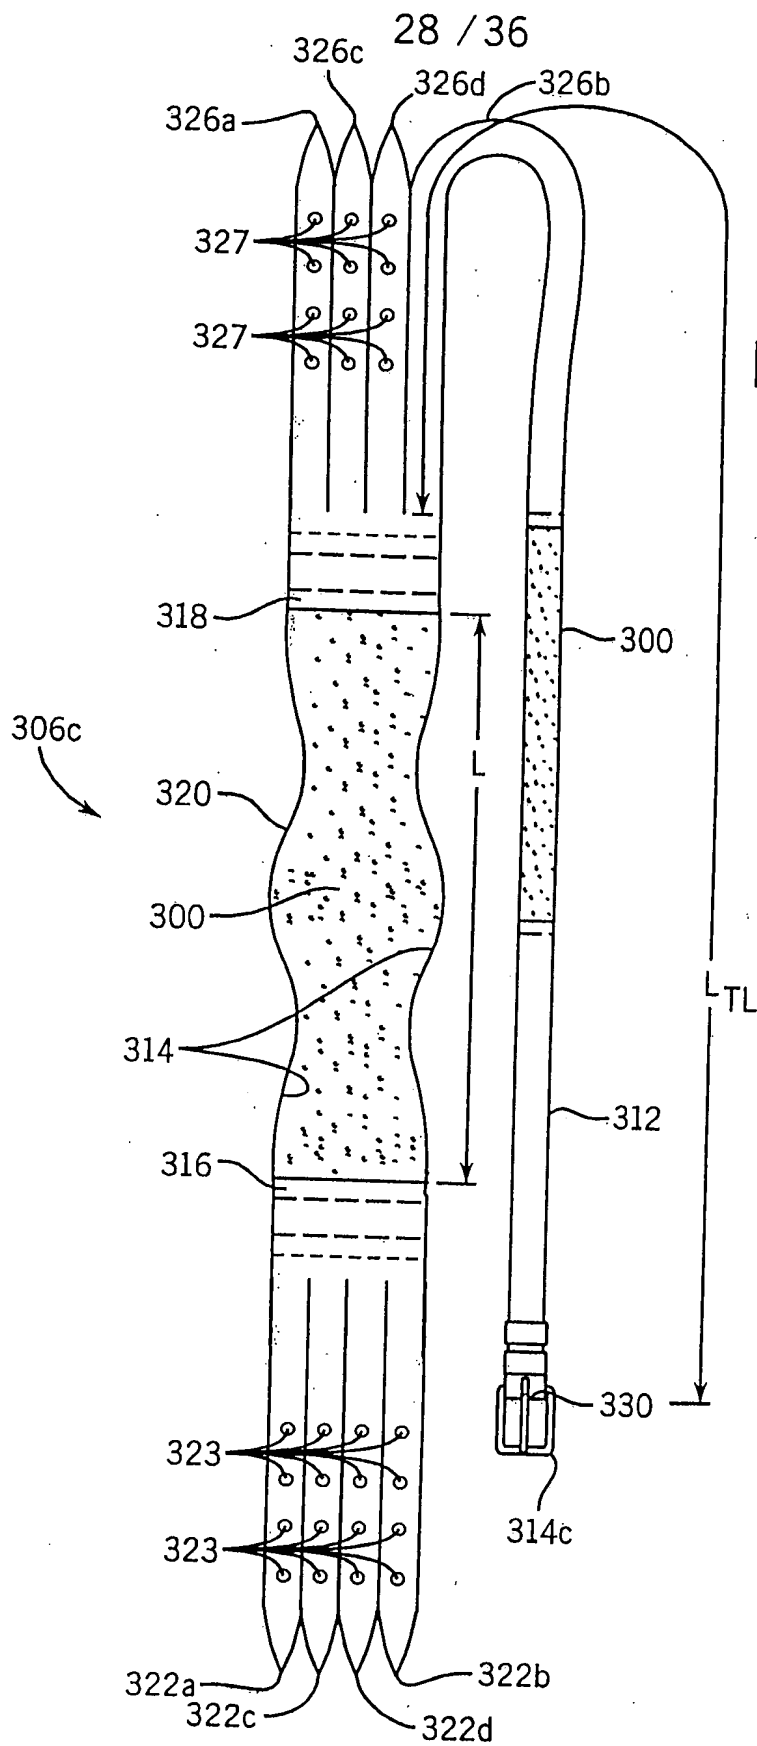


FIG. 41



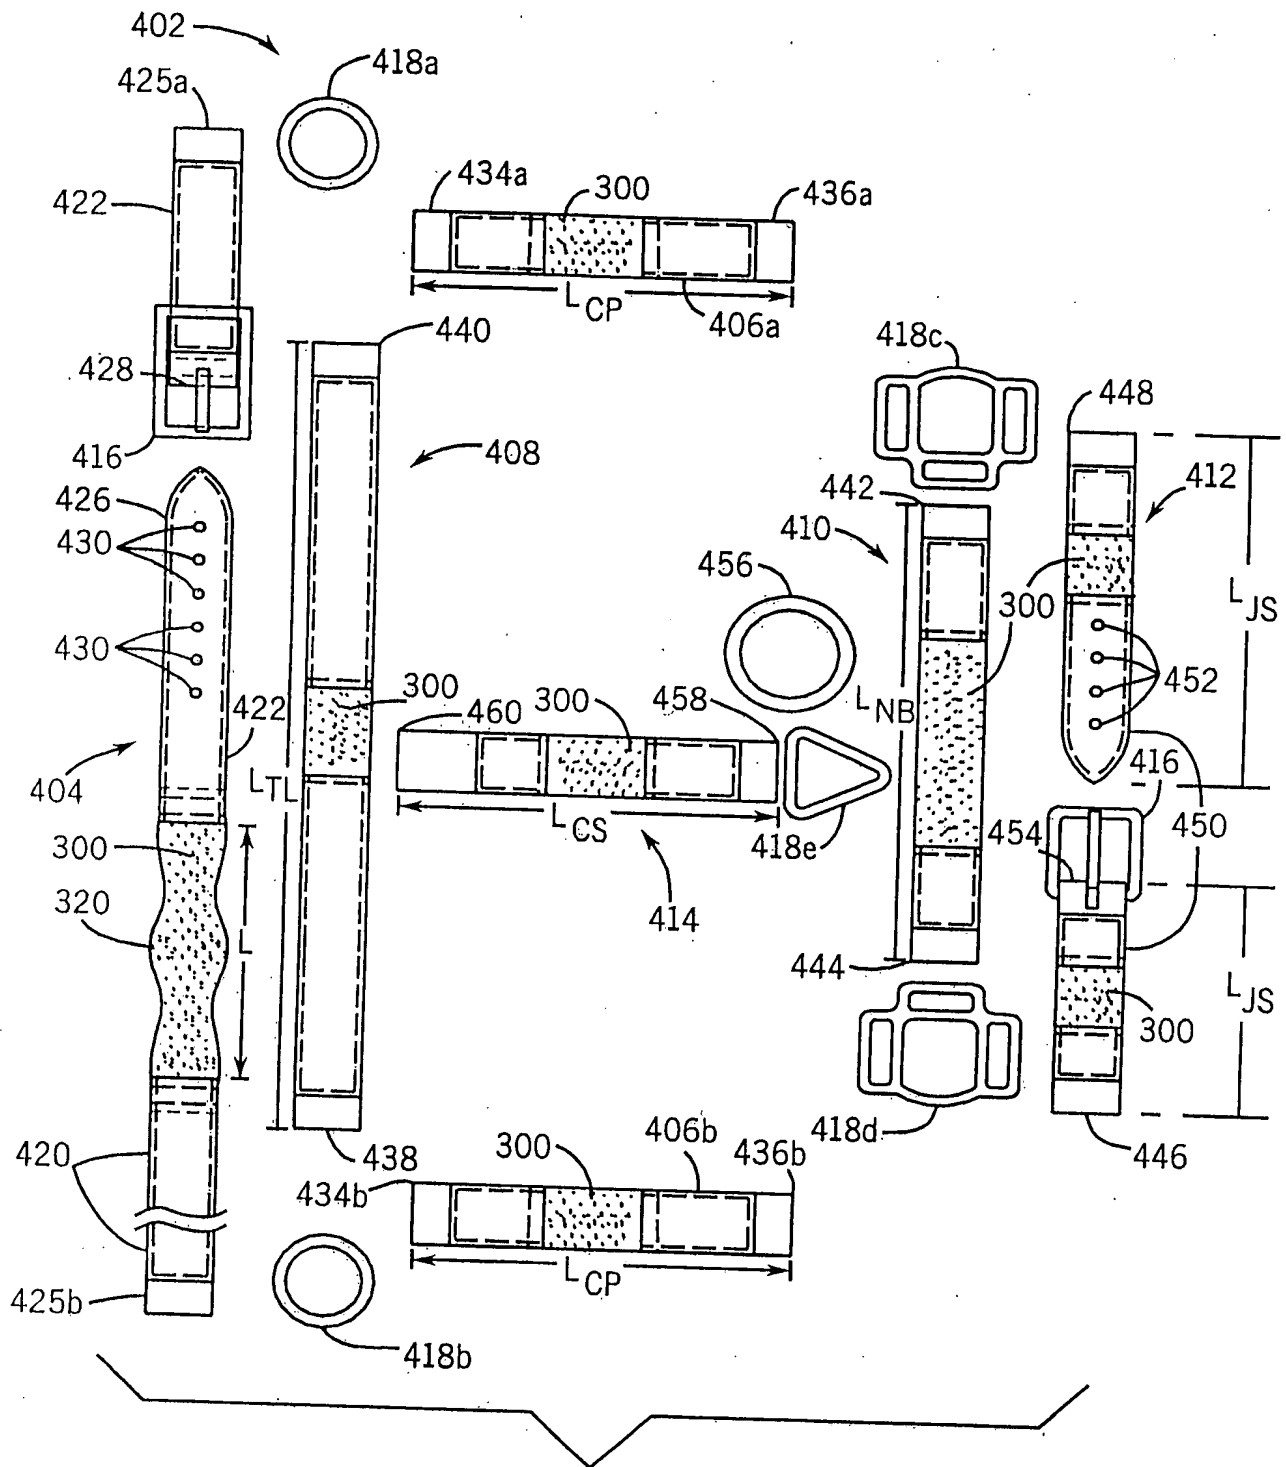


FIG. 43

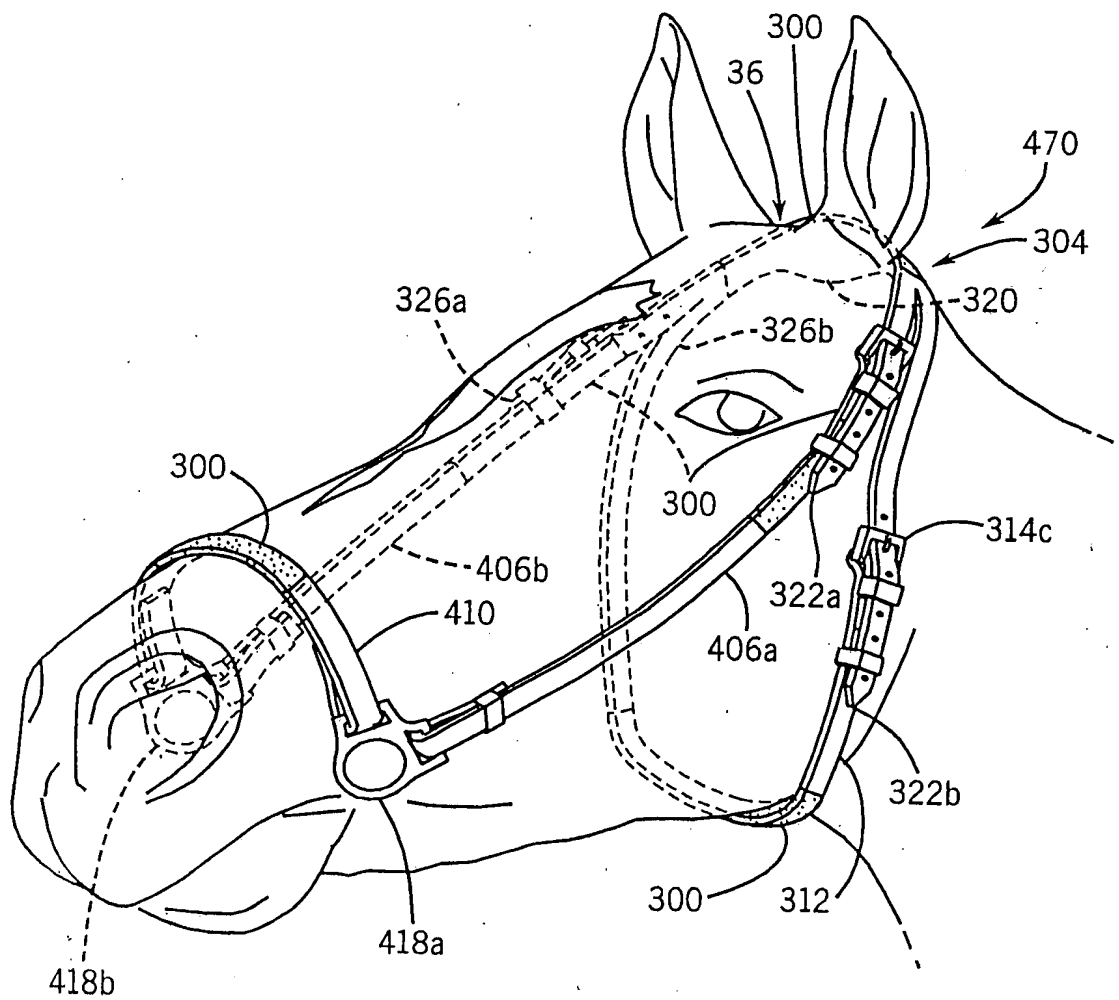


FIG. 44

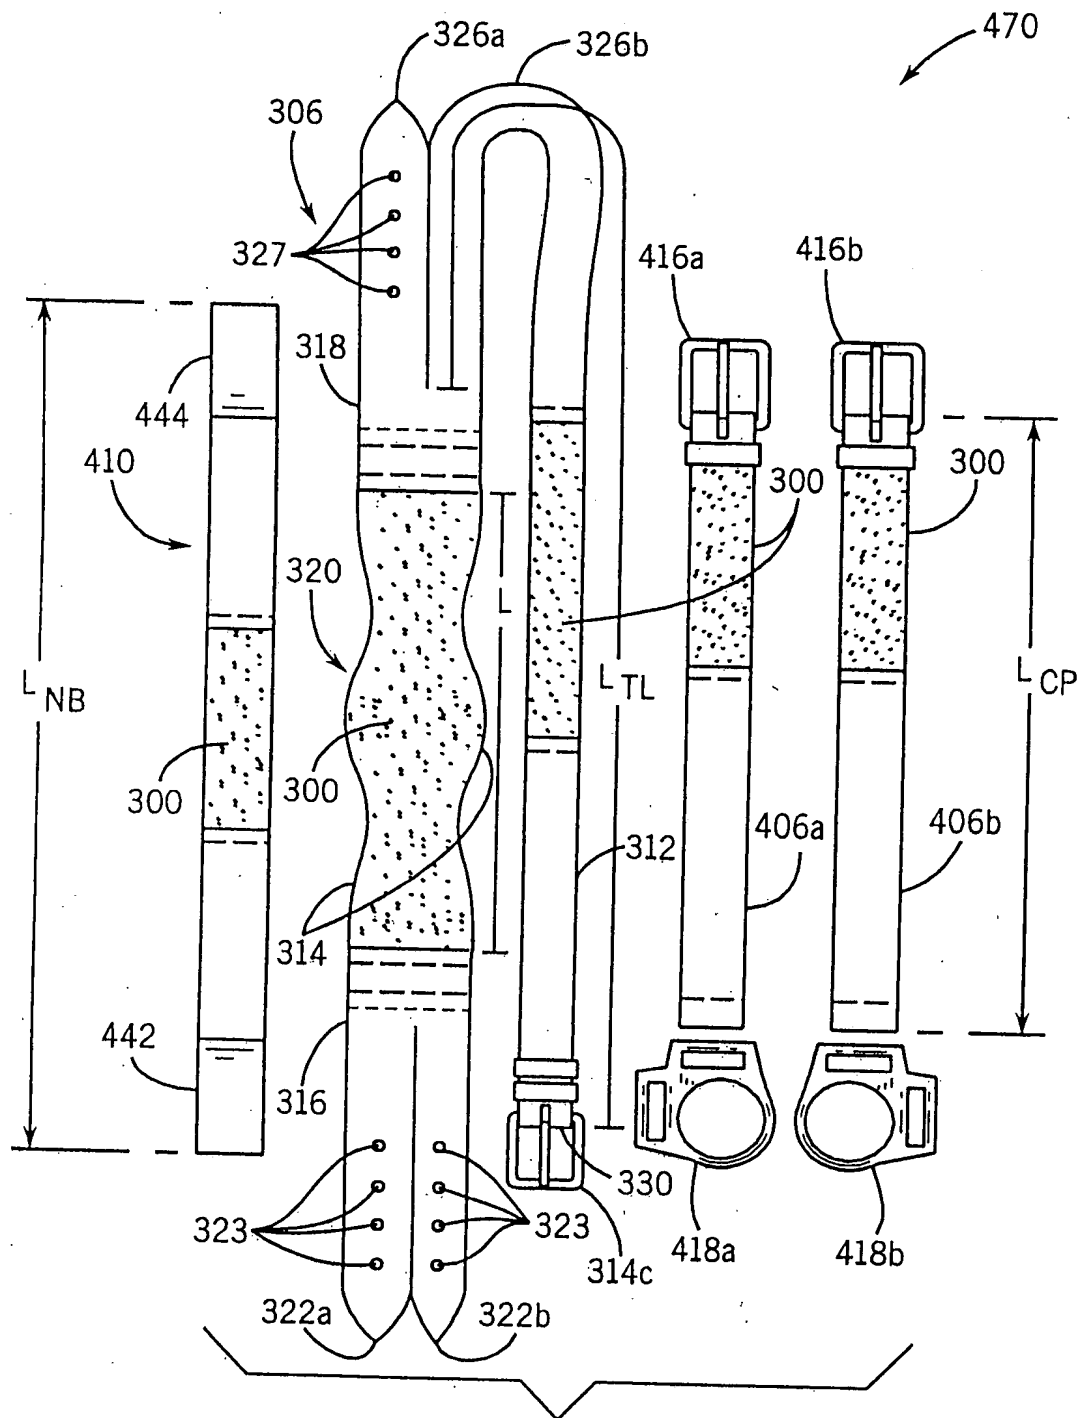


FIG. 45



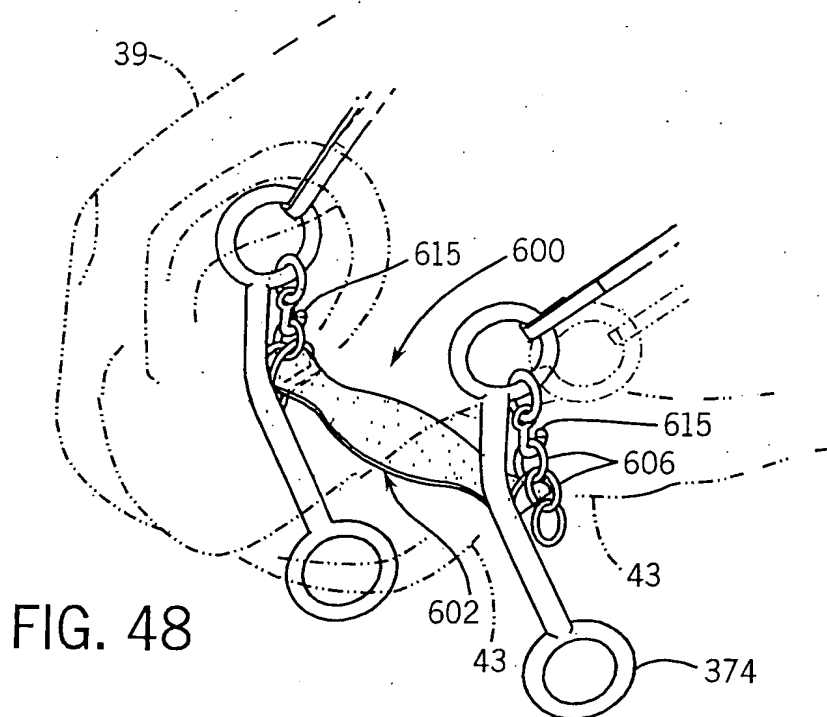


FIG. 48

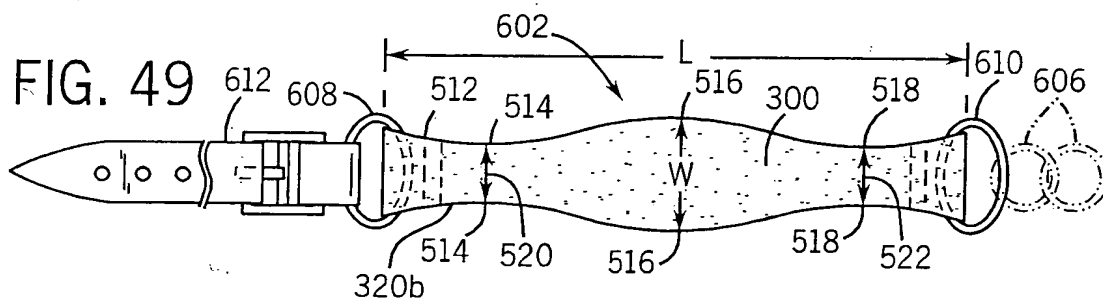


FIG. 49

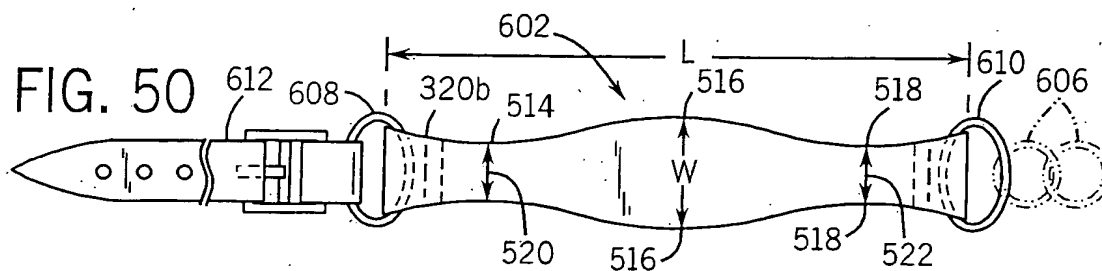


FIG. 50

